

# Technical Information

## Proline Promag H 10

Electromagnetic flowmeter



Flowmeter for hygienic basic applications with simple operating concept

### Application

- The bidirectional measuring principle is virtually independent of pressure, density, temperature and viscosity
- For applications with hygienic requirements

### Device properties

- Liner made of PFA
- Sensor housing made of stainless steel (3-A, EHEDG)
- Wetted materials CIP/SIP cleanable
- System integration with HART, Modbus RS485
- Flexible operation with app and optional display

### Your benefits

- Flexible installation concept – numerous hygienic process connections
- Energy-saving flow measurement – no pressure loss due to cross-section constriction
- Maintenance-free – no moving parts
- Optimum usability – operation with mobile devices and SmartBlue App or touch screen display
- Easy, time-saving commissioning – guided parameter configuration in advance and in the field
- Integrated verification – Heartbeat Technology

## Table of contents

<b>About this document</b>	<b>4</b>	<b>Process</b>	<b>48</b>
Symbols used	4	Medium temperature range	48
Associated documentation	4	Conductivity	48
Ordering information	4	Flow limit	48
Registered trademarks	6	Pressure-temperature ratings	50
		Pressure tightness	52
		Pressure loss	52
<b>Function and system design</b>	<b>8</b>	<b>Mechanical construction</b>	<b>54</b>
Measuring principle	8	Weight	54
Product design	8	Measuring pipe specification	54
IT security	9	Materials	55
Device-specific IT security	9	Fitted electrodes	56
		Surface roughness	56
<b>Input</b>	<b>12</b>	<b>Dimensions in SI units</b>	<b>58</b>
Measured variable	12	Compact version	58
Operable flow range	12	Remote version	59
Measuring range	12	Sensor flange connection	61
		Flange connections	63
<b>Output</b>	<b>16</b>	Clamp connections	66
Output versions	16	Welding socket	67
Output signal	16	Couplings	69
Signal on alarm	19	Mounting kit	72
Low flow cut off	19	Accessories	73
Galvanic isolation	19		
Protocol-specific data	19	<b>Dimensions in US units</b>	<b>78</b>
		Compact version	78
<b>Power supply</b>	<b>22</b>	Remote version	79
Terminal assignment	22	Sensor flange connection	81
Supply voltage	22	Flange connections	83
Power consumption	22	Clamp connections	83
Current consumption	22	Welding socket	84
Power supply failure	23	Mounting kits	85
Electrical connection	23	Accessories	86
Potential equalization	27		
Terminals	28	<b>Local display</b>	<b>90</b>
Cable entries	28	Operating concept	90
		Operating options	90
<b>Cable specification</b>	<b>30</b>	Operating tools	91
Requirements for connecting cable	30		
Ground cable requirements	30	<b>Certificates and approvals</b>	<b>94</b>
Connecting cable requirements	30	Non-Ex approval	94
		Pressure Equipment Directive	94
<b>Performance characteristics</b>	<b>34</b>	Pharmaceutical compatibility	94
Reference operating conditions	34	HART certification	94
Maximum measured error	34	Radio approval	94
Repeatability	34	Other standards and guidelines	94
Temperature measurement response time	35		
Influence of ambient temperature	35	<b>Application packages</b>	<b>98</b>
		Use	98
<b>Installation</b>	<b>38</b>	Heartbeat Verification + Monitoring	98
Installation conditions	38		
		<b>Accessories</b>	<b>100</b>
<b>Environment</b>	<b>44</b>	Device-specific accessories	100
Ambient temperature range	44	Communication-specific accessories	101
Storage temperature	44	Service-specific accessory	101
Degree of protection	44	System components	102
Vibration-resistance and shock-resistance	44		
Interior cleaning	45		
Electromagnetic compatibility (EMC)	45		

## About this document

---

Symbols used	4
Associated documentation	4
Ordering information	4
Registered trademarks	6

## Symbols used

### Electronics

-  Direct current
-  Alternating current
-  Direct current and alternating current
-  Protective earthing

### Types of information

-  Preferred procedures, processes or actions
-  Permitted procedures, processes or actions
-  Forbidden procedures, processes or actions
-  Additional information
-  Reference to documentation
-  Reference to page
-  Reference to graphic

### Explosion protection

-  Hazardous area
-  Non-hazardous area

## Associated documentation

Technical Information	Overview of the device with the most important technical data.
Operating Instructions	All the information that is required in the various phases of the life cycle of the device: from product identification, incoming acceptance and storage, to mounting, connection, operation and commissioning through to troubleshooting, maintenance and disposal as well as the technical data and dimensions.
Sensor Brief Operating Instructions	Incoming acceptance, transport, storage and mounting of the device.
Transmitter Brief Operating Instructions	Electrical connection and commissioning of the device.
Description of Parameters	Detailed explanation of the menus and parameters.
Safety Instructions	Documents for the use of the device in hazardous areas.
Special Documentation	Documents with more detailed information on specific topics.
Installation Instructions	Installation of spare parts and accessories.



The device documentation is available online on the device product page and in the Downloads area: [www.endress.com](http://www.endress.com)

## Ordering information

Detailed ordering information is available for your nearest sales organization [www.addresses.endress.com](http://www.addresses.endress.com) or in the Product Configurator under [www.endress.com](http://www.endress.com) :

1. Click Corporate
2. Select the country
3. Click Products
4. Select the product using the filters and search field
5. Open the product page

The Configuration button to the right of the product image opens the Product Configurator.



**Product Configurator - the tool for individual product configuration**

- Up-to-the-minute configuration data
- Depending on the device: Direct input of measuring point-specific information such as measuring range or operating language
- Automatic verification of exclusion criteria
- Automatic creation of the order code and its breakdown in PDF or Excel output format
- Ability to order directly in the Endress+Hauser Online Shop

### Registered trademarks

#### **HART®**

Registered trademark of the FieldComm Group, Austin, USA

#### **Modbus®**

Registered trademark of SCHNEIDER AUTOMATION, INC.

#### **Bluetooth®**

The Bluetooth word mark and Bluetooth logos are registered trademarks of Bluetooth SIG, Inc. and any use of such marks by Endress+Hauser is under license. Other trademarks and trade names are those of their respective owners.

#### **Apple®**

Apple, the Apple logo, iPhone, and iPod touch are trademarks of Apple Inc., registered in the U.S. and other countries. App Store is a service mark of Apple Inc.

#### **Android®**

Android, Google Play and the Google Play logo are trademarks of Google Inc.


## Function and system design

---

Measuring principle	8
Product design	8
IT security	9
Device-specific IT security	9

## Measuring principle

Following *Faraday's law of magnetic induction*, a voltage is induced in a conductor moving through a magnetic field.

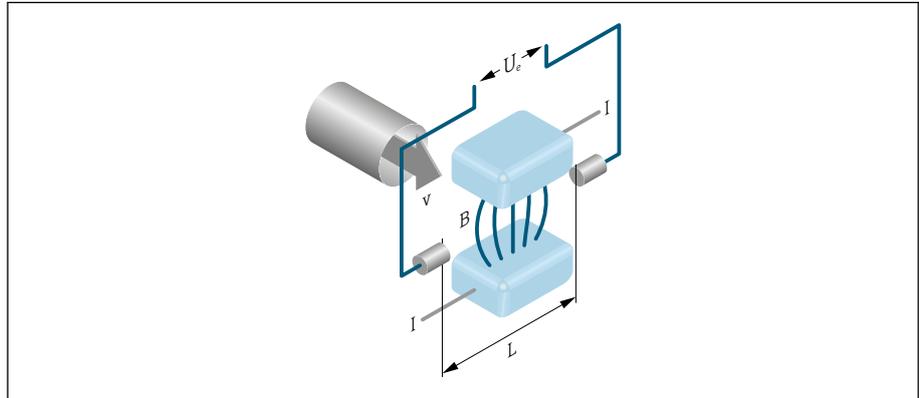

A0028962

- U<sub>e</sub>* Induced voltage  
*B* Magnetic induction (magnetic field)  
*L* Electrode spacing  
*I* Current  
*v* Flow velocity

In the electromagnetic measuring principle, the flowing medium is the moving conductor. The voltage induced ( $U_e$ ) is proportional to the flow velocity ( $v$ ) and is supplied to the amplifier by means of two measuring electrodes. The flow volume ( $Q$ ) is calculated via the pipe cross-section ( $A$ ). The DC magnetic field is created through a switched direct current of alternating polarity.

### Formulae for calculation

- Induced voltage  $U_e = B \cdot L \cdot v$
- Volume flow  $Q = A \cdot v$

## Product design


The device consists of a transmitter and a sensor.

Two device versions are available:

- Compact version – transmitter and sensor form a mechanical unit.
- Remote version - transmitter and sensor are mounted in separate locations.

### Compact version

The transmitter and sensor form a mechanical unit.

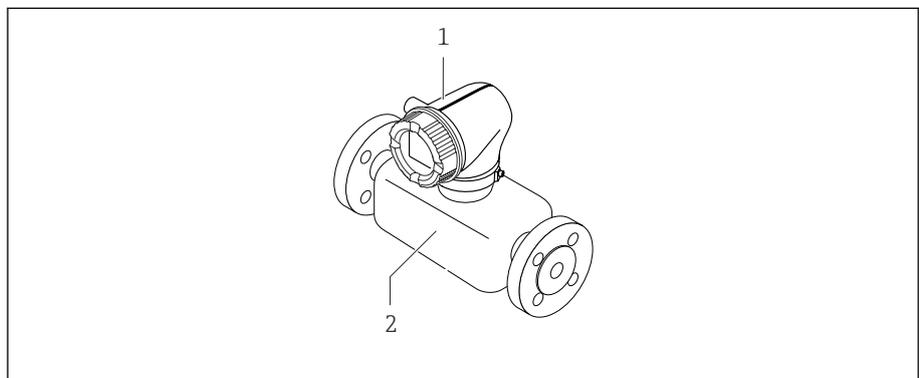


A0008262

- 1 Transmitter  
 2 Sensor

### Remote version

The transmitter and sensor are mounted in physically separate locations.

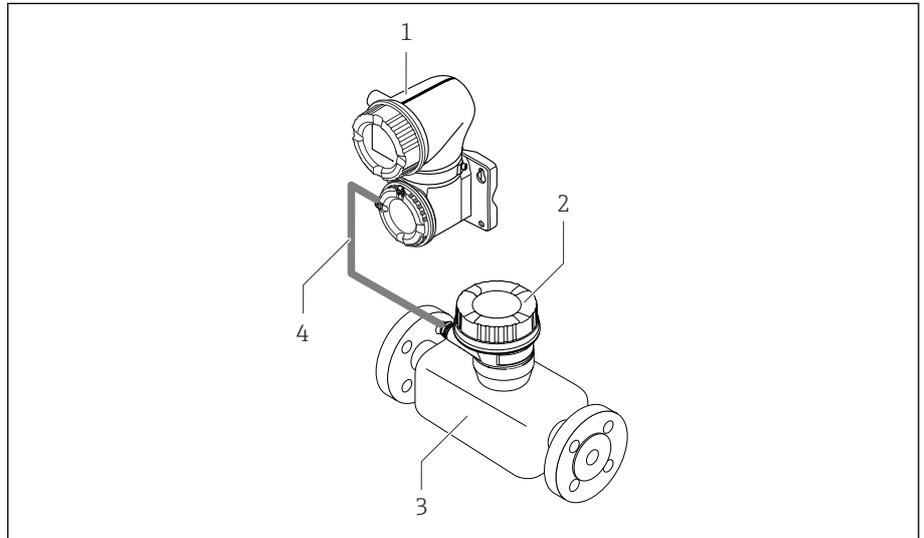

A0028196

- 1 Transmitter
- 2 Sensor connection housing
- 3 Sensor
- 4 Connecting cable

### Measuring system

Proline 10 transmitter	Promag H sensor	
	DN 2 to 25 mm ( $\frac{1}{12}$ to 1 in)	DN > 25 mm (1 in)

### IT security

We only provide a warranty if the device is installed and used as described in the Operating Instructions. The device is equipped with security mechanisms to protect it against any inadvertent changes to the device settings.

IT security measures in line with operators' security standards and designed to provide additional protection for the device and device data transfer must be implemented by the operators themselves.

### Device-specific IT security

#### Access via Bluetooth

Secure signal transmission via Bluetooth uses an encryption method tested by the Fraunhofer Institute.

- Without the SmartBlue App, the device is not visible via Bluetooth.
- Only one point-to-point connection is established between the device and a smartphone or tablet.

### Access via the SmartBlue App

Two access levels (user roles) are defined for the device: the **Operator** user role and the **Maintenance** user role. The **Maintenance** user role is configured when the device leaves the factory.

If a user-specific access code is not defined (in the Enter access code parameter), the default setting **0000** continues to apply and the **Maintenance** user role is automatically enabled. The device's configuration data are not write-protected and can be edited at all times.

If a user-specific access code has been defined (in the Enter access code parameter), all the parameters are write-protected. The device is accessed with the **Operator** user role. When the user-specific access code is entered a second time, the **Maintenance** user role is enabled. All parameters can be written to.



For detailed information, see the "Description of Device Parameters" document pertaining to the device.

### Protecting access via a password

There are a variety of ways to protect against write access to the device parameters:

- User-specific access code:  
Protect write access to the device parameters via all the interfaces.
- Bluetooth key:  
The password protects access and the connection between an operating unit, e.g. a smartphone or tablet, and the device via the Bluetooth interface.

#### General notes on the use of passwords

- The access code and Bluetooth key supplied with the device must be defined during commissioning.
- Follow the general rules for generating a secure password when defining and managing the access code and Bluetooth key.
- The user is responsible for the management and careful handling of the access code and Bluetooth key.

### Write protection switch

The entire operating menu can be locked via the write protection switch. The values of the parameters cannot be changed. Write protection is disabled when the device leaves the factory.

Write protection is enabled with the write protection switch on the back of the display module.

## Input

---

Measured variable	12
Operable flow range	12
Measuring range	12

### Measured variable

Direct measured variables	<ul style="list-style-type: none"> <li>▪ Volume flow (proportional to induced voltage)</li> <li>▪ Conductivity (order code for "Sensor Option", option CX)</li> <li>▪ Temperature (DN 15 to 150 (½" to 6") with order code for "Sensor option", option CI "Medium temperature measurement" )</li> </ul>
Calculated measured variables	<ul style="list-style-type: none"> <li>▪ Mass flow</li> <li>▪ Corrected conductivity (DN 15 to 150 (½" to 6") with order code for "Sensor option", option CI "Medium temperature measurement" and order code for "Functionality", option D)</li> </ul>

### Operable flow range

Over 1000 : 1

### Measuring range

Typically  $v = 0.01$  to  $10$  m/s ( $0.03$  to  $33$  ft/s) with the specified accuracy

Electrical conductivity:  $\geq 5$   $\mu\text{S/cm}$  for liquids in general

Flow characteristic values in SI units: DN 2 to 150 (½" to 6")

Nominal diameter		Recommended flow min./max. full scale value ( $v \sim 0.3/10$ m/s)	Full scale value current output ( $v \sim 2.5$ m/s)	Factory settings	
[mm]	[in]			Pulse value ( $\sim 2$ pulse/s)	Low flow cut off ( $v \sim 0.04$ m/s)
		[dm <sup>3</sup> /min]	[dm <sup>3</sup> /min]	[dm <sup>3</sup> ]	[dm <sup>3</sup> /min]
2	½ <sub>12</sub>	0.06 to 1.8	0.5	0.005	0.01
4	⅝ <sub>32</sub>	0.25 to 7	2	0.025	0.05
8	⅝ <sub>16</sub>	1 to 30	8	0.1	0.1
15	½	4 to 100	25	0.2	0.5
25	1	9 to 300	75	0.5	1
40	1 ½	25 to 700	200	1.5	3
50	2	35 to 1 100	300	2.5	5
65	–	60 to 2 000	500	5	8
80	3	90 to 3 000	750	5	12
100	4	145 to 4 700	1 200	10	20
125	5	220 to 7 500	1 850	15	30
150	6	330 to 10 000	2 500	30	42

Flow characteristic values in US units: ½" - 6" (DN 2 - 150)

Nominal diameter		Recommended flow min./max. full scale value ( $v \sim 0.3/10$ m/s)	Full scale value current output ( $v \sim 2.5$ m/s)	Factory settings	
[in]	[mm]			Pulse value ( $\sim 2$ pulse/s)	Low flow cut off ( $v \sim 0.04$ m/s)
		[gal/min]	[gal/min]	[gal]	[gal/min]
½ <sub>12</sub>	2	0.015 to 0.5	0.1	0.001	0.002
⅝ <sub>32</sub>	4	0.07 to 2	0.5	0.005	0.008
⅝ <sub>16</sub>	8	0.25 to 8	2	0.02	0.025
½	15	1 to 27	6	0.05	0.1

Nominal diameter		Recommended flow min./max. full scale value (v ~ 0.3/10 m/s)	Full scale value current output (v ~ 2.5 m/s)	Factory settings	
[in]	[mm]			Pulse value (~ 2 pulse/s)	Low flow cut off (v ~ 0.04 m/s)
		[gal/min]	[gal/min]	[gal]	[gal/min]
1	25	2.5 to 80	18	0.2	0.25
1 ½	40	7 to 190	50	0.5	0.75
2	50	10 to 300	75	0.5	1.25
3	80	24 to 800	200	2	2.5
4	100	40 to 1250	300	2	4
5	125	60 to 1950	450	5	7
6	150	90 to 2650	600	5	12

---

## Output

---

Output versions	16
Output signal	16
Signal on alarm	19
Low flow cut off	19
Galvanic isolation	19
Protocol-specific data	19

## Output versions

Order code for 020: output; input	Output version
Option B	<ul style="list-style-type: none"> <li>■ Current output 4 to 20 mA HART</li> <li>■ Pulse/frequency/switch output</li> </ul>
Option M	<ul style="list-style-type: none"> <li>■ Modbus RS485</li> <li>■ Current output 4 to 20 mA</li> </ul>

## Output signal

### Current output 4 to 20 mA HART

Signal mode	Choose via terminal assignment: <ul style="list-style-type: none"> <li>■ Active</li> <li>■ Passive</li> </ul>
Current range	Can be set to: <ul style="list-style-type: none"> <li>■ 4 to 20 mA NAMUR</li> <li>■ 4 to 20 mA US</li> <li>■ 4 to 20 mA</li> <li>■ Fixed current</li> </ul>
Max. output current	21.5 mA
Open-circuit voltage	DC < 28.8 V (active)
Max. input voltage	DC 30 V (passive)
Max. load	400 Ω
Resolution	1 μA
Damping	Configurable: 0 to 999.9 s
Assignable measured variables	<ul style="list-style-type: none"> <li>■ Off</li> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Temperature*</li> <li>■ Flow velocity</li> <li>■ Conductivity*</li> <li>■ Corrected conductivity*</li> <li>■ Electronic temperature</li> <li>■ Noise*</li> <li>■ Coil current shot time*</li> <li>■ Reference electrode potential against PE*</li> </ul> <p>* Visibility depends on order options or device settings</p>

### Modbus RS485

Physical interface	RS485 in accordance with EIA/TIA-485 standard
--------------------	---

### Current output 4 to 20 mA

Signal mode	Choose via terminal assignment: <ul style="list-style-type: none"> <li>■ Active</li> <li>■ Passive</li> </ul>
Current range	Can be set to: <ul style="list-style-type: none"> <li>■ 4 to 20 mA NAMUR</li> <li>■ 4 to 20 mA US</li> <li>■ 4 to 20 mA</li> <li>■ Fixed current</li> </ul>

<b>Max. output current</b>	21.5 mA
<b>Open-circuit voltage</b>	DC < 28.8 V (active)
<b>Max. input voltage</b>	DC 30 V (passive)
<b>Max. load</b>	400 Ω
<b>Resolution</b>	1 μA
<b>Damping</b>	Configurable: 0 to 999.9 s
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>▪ Off</li> <li>▪ Volume flow</li> <li>▪ Mass flow</li> <li>▪ Temperature*</li> <li>▪ Flow velocity</li> <li>▪ Conductivity*</li> <li>▪ Corrected conductivity*</li> <li>▪ Electronic temperature</li> <li>▪ Noise*</li> <li>▪ Coil current shot time*</li> <li>▪ Reference electrode potential against PE*</li> </ul> <p>* Visibility depends on order options or device settings</p>

#### Pulse/frequency/switch output

<b>Function</b>	Can be set to: <ul style="list-style-type: none"> <li>▪ Pulse output</li> <li>▪ Frequency output</li> <li>▪ Switch output</li> </ul>
<b>Version</b>	Open collector: Passive
<b>Input values</b>	<ul style="list-style-type: none"> <li>▪ DC 10.4 to 30 V</li> <li>▪ Max. 140 mA</li> </ul>
<b>Voltage drop</b>	<ul style="list-style-type: none"> <li>▪ ≤ DC 2 V @ 100 mA</li> <li>▪ ≤ DC 2.5 V @ max. input current</li> </ul>

<b>Pulse output</b>	
<b>Pulse width</b>	Configurable: 0.05 to 2 000 ms
<b>Max. pulse rate</b>	10 000 Impulse/s
<b>Pulse value</b>	Configurable
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>▪ Volume flow</li> <li>▪ Mass flow</li> </ul>

<b>Frequency output</b>	
<b>Output frequency</b>	Configurable: end value frequency 2 to 10 000 Hz ( $f_{\max} = 12\,500$ Hz)
<b>Damping</b>	Configurable: 0 to 999.9 s

<b>Pulse/pause ratio</b>	1:1
<b>Assignable measured variables</b>	<ul style="list-style-type: none"> <li>■ Off</li> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Temperature*</li> <li>■ Flow velocity</li> <li>■ Conductivity*</li> <li>■ Corrected conductivity*</li> <li>■ Electronic temperature</li> <li>■ Noise*</li> <li>■ Coil current shot time*</li> <li>■ Reference electrode potential against PE*</li> </ul> <p>* Visibility depends on order options or device settings</p>

<b>Switch output</b>	
<b>Switching behavior</b>	Binary, conductive or non-conductive
<b>Switching delay</b>	Configurable: 0 to 100 s
<b>Number of switching cycles</b>	Unlimited
<b>Assignable functions</b>	<ul style="list-style-type: none"> <li>■ Off</li> <li>■ On</li> <li>■ Diagnostic behavior: <ul style="list-style-type: none"> <li>■ Alarm</li> <li>■ Warning</li> <li>■ Warning and alarm</li> </ul> </li> <li>■ Limit value: <ul style="list-style-type: none"> <li>■ Off</li> <li>■ Volume flow</li> <li>■ Mass flow</li> <li>■ Temperature*</li> <li>■ Flow velocity</li> <li>■ Conductivity*</li> <li>■ Corrected conductivity*</li> <li>■ Totalizer 1...3</li> <li>■ Electronic temperature</li> </ul> </li> <li>■ Flow direction monitoring</li> <li>■ Status <ul style="list-style-type: none"> <li>■ Empty pipe detection</li> <li>■ Low flow cut off</li> </ul> </li> </ul> <p>* Visibility depends on order options or device settings</p>

### Signal on alarm

Output behavior in the event of a device alarm (failure mode)

#### HART

<b>Device diagnostics</b>	Device condition can be read out via HART Command 48
---------------------------	--

#### Modbus RS485

<b>Failure mode</b>	Selectable: <ul style="list-style-type: none"> <li>▪ NaN value instead of current value</li> <li>▪ Last valid value</li> </ul>
---------------------	--

#### Current output 4 to 20 mA

<b>4 to 20 mA</b>	Selectable: <ul style="list-style-type: none"> <li>▪ Min. value: 3.59 mA</li> <li>▪ Max. value: 21.5 mA</li> <li>▪ Freely definable value between: 3.59 to 21.5 mA</li> <li>▪ Actual value</li> <li>▪ Last valid value</li> </ul>
-------------------	---

#### Pulse/frequency/switch output

<b>Pulse output</b>	Selectable: <ul style="list-style-type: none"> <li>▪ Actual value</li> <li>▪ No pulses</li> </ul>
<b>Frequency output</b>	Selectable: <ul style="list-style-type: none"> <li>▪ Actual value</li> <li>▪ 0 Hz</li> <li>▪ Defined value: 0 to 12 500 Hz</li> </ul>
<b>Switch output</b>	Selectable: <ul style="list-style-type: none"> <li>▪ Current status</li> <li>▪ Open</li> <li>▪ Closed</li> </ul>

#### Low flow cut off

The switch points for low flow cut off are user-selectable.

#### Galvanic isolation

The outputs are galvanically isolated from one another and from earth.

#### Protocol-specific data

##### HART

<b>Bus structure</b>	The HART signal overlays the 4 to 20 mA current output.
<b>Manufacturer ID</b>	0x11
<b>Device type ID</b>	0x71
<b>HART protocol revision</b>	7
<b>Device description files (DTM, DD)</b>	Information and files under: <a href="http://www.endress.com">www.endress.com</a>

<b>HART load</b>	At least 250 Ω
<b>System integration</b>	Measured variables via HART protocol

### Modbus RS485

<b>Physical interface</b>	RS485 in accordance with EIA/TIA-485 standard
<b>Terminating resistor</b>	Not integrated
<b>Protocol</b>	Modbus Applications Protocol Specification V1.1
<b>Response times</b>	<ul style="list-style-type: none"> <li>▪ Direct data access: typically 25 to 50 ms</li> <li>▪ Auto-scan buffer (data range): typically 3 to 5 ms</li> </ul>
<b>Device type</b>	Slave
<b>Slave address range</b>	1 to 247
<b>Broadcast address range</b>	0
<b>Function codes</b>	<ul style="list-style-type: none"> <li>▪ 03: Read holding register</li> <li>▪ 04: Read input register</li> <li>▪ 06: Write single registers</li> <li>▪ 08: Diagnostics</li> <li>▪ 16: Write multiple registers</li> <li>▪ 23: Read/write multiple registers</li> </ul>
<b>Broadcast messages</b>	Supported by the following function codes: <ul style="list-style-type: none"> <li>▪ 06: Write single registers</li> <li>▪ 16: Write multiple registers</li> <li>▪ 23: Read/write multiple registers</li> </ul>
<b>Supported baud rate</b>	<ul style="list-style-type: none"> <li>▪ 1 200 BAUD</li> <li>▪ 2 400 BAUD</li> <li>▪ 4 800 BAUD</li> <li>▪ 9 600 BAUD</li> <li>▪ 19 200 BAUD</li> <li>▪ 38 400 BAUD</li> <li>▪ 57 600 BAUD</li> <li>▪ 115 200 BAUD</li> </ul>
<b>Data transfer mode</b>	RTU
<b>Data access</b>	Each parameter can be accessed via Modbus RS485.  For Modbus register information
<b>System integration</b>	Information on system integration . <ul style="list-style-type: none"> <li>▪ Modbus RS485 information</li> <li>▪ Function codes</li> <li>▪ Register information</li> <li>▪ Response time</li> <li>▪ Modbus data map</li> </ul>

## Power supply

---

Terminal assignment	22
Supply voltage	22
Power consumption	22
Current consumption	22
Power supply failure	23
Electrical connection	23
Potential equalization	27
Terminals	28
Cable entries	28

## Terminal assignment

 The terminal assignment is documented on an adhesive label.

The following terminal assignment is available:

*Current output 4 to 20 mA HART (active) and pulse/frequency/switch output*

Supply voltage		Output 1				Output 2	
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)
L/+	N/-	Current output 4 to 20 mA HART (active)		-		Pulse/frequency/switch output (passive)	

*Current output 4 to 20 mA HART (passive) and pulse/frequency/switch output*

Supply voltage		Output 1				Output 2	
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (+)	23 (-)
L/+	N/-	-		Current output 4 to 20 mA HART (passive)		Pulse/frequency/switch output (passive)	

*Modbus RS485 and current output 4 to 20 mA (active)*

Supply voltage		Output 1				Output 2	
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (B)	23 (A)
L/+	N/-	Current output 4 to 20 mA (active)		-		Modbus RS485	

*Modbus RS485 and current output 4 to 20 mA (passive)*

Supply voltage		Output 1				Output 2	
1 (+)	2 (-)	26 (+)	27 (-)	24 (+)	25 (-)	22 (B)	23 (A)
L/+	N/-	-		Current output 4 to 20 mA (passive)		Modbus RS485	

## Supply voltage

Order code for "Power supply"	Terminal voltage	Frequency range
Option D	DC 24 V	-20 to +30 %
Option E	AC 100 to 240 V	-15 to +10 %
Option I	DC 24 V	-20 to +30 %
	AC 100 to 240 V	-15 to +10 %
Option M non-hazardous area	DC 24 V	-20 to +30 %
	AC 100 to 240 V	-15 to +10 %

## Power consumption

- Transmitter: max. 10 W (active power)
- Switch-on current: max. 36 A (< 5 ms) as per NAMUR Recommendation NE 21

## Current consumption


- Max. 400 mA (24 V)
- Max. 200 mA (110 V, 50/60 Hz; 230 V, 50/60 Hz)

### Power supply failure

- Totalizers stop at the last value measured.
- Device configuration remains unchanged.
- Error messages (incl. total operated hours) are stored.

### Electrical connection


#### Connections and terminal assignment, remote version connecting cable

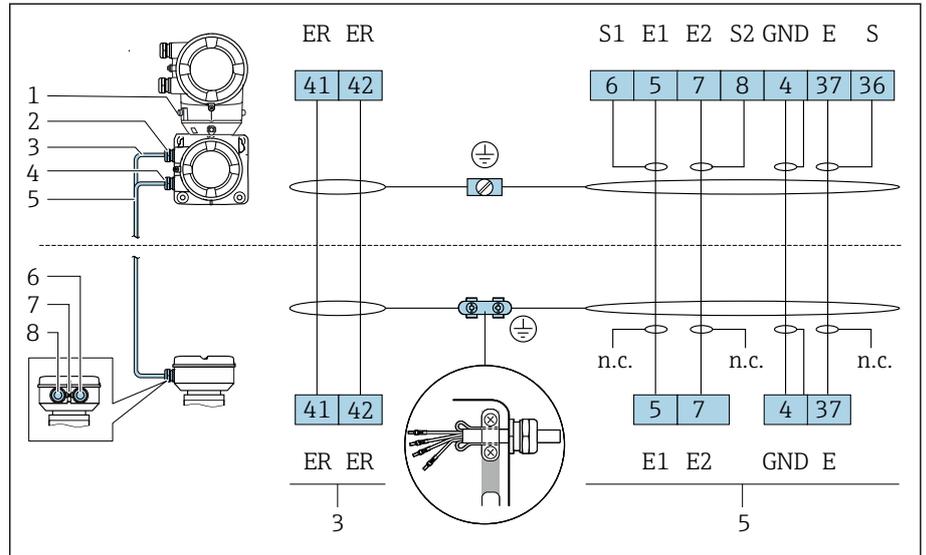

- 1 Ground terminal, outer
- 2 Transmitter housing: cable entry for coil current cable
- 3 Coil current cable
- 4 Transmitter housing: cable entry for electrode cable
- 5 Electrode cable
- 6 Sensor connection housing: cable entry for electrode cable
- 7 Ground terminal, outer
- 8 Sensor connection housing: cable entry for coil current cable

#### Transmitter terminal connections


**i** Terminal assignment → *Terminal assignment*, 22

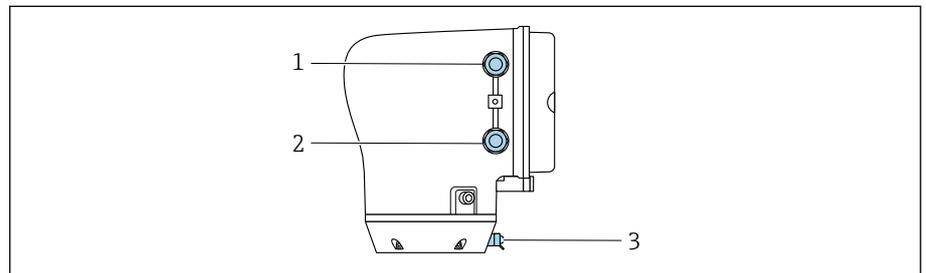

- 1 Cable entry for power supply cable: supply voltage
- 2 Cable entry for signal cable
- 3 Ground terminal, outer

### Examples for electric terminals


#### Current output 4 to 20 mA HART (active)

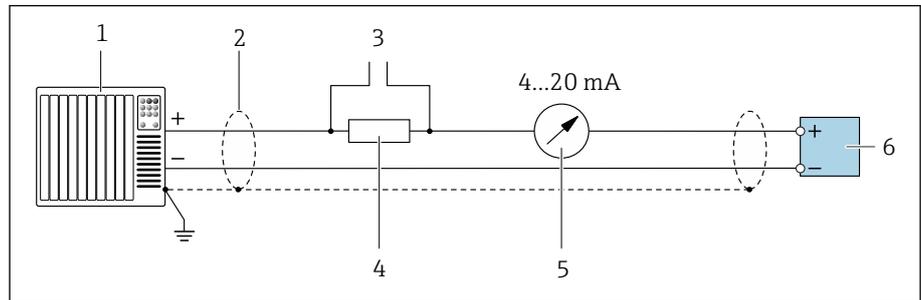

A0029055

- 1 Automation system with current input, e.g. PLC
- 2 Cable shield
- 3 Connection for HART operating devices
- 4 Resistor for HART communication ( $\geq 250 \Omega$ ); observe max. load.
- 5 Analog display unit; observe max. load.
- 6 Transmitter


#### Current output 4 to 20 mA HART (passive)

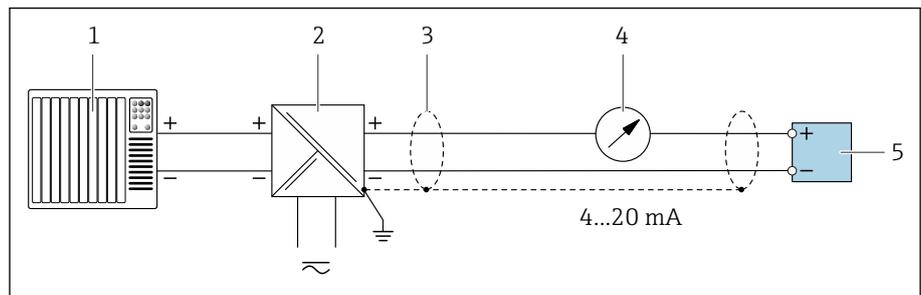

A0028762

- 1 Automation system with current input, e.g. PLC
- 2 Active barrier for supply voltage, e.g. RN221N
- 3 Cable shield
- 4 Analog display unit; observe max. load.
- 5 Transmitter

HART input (passive)

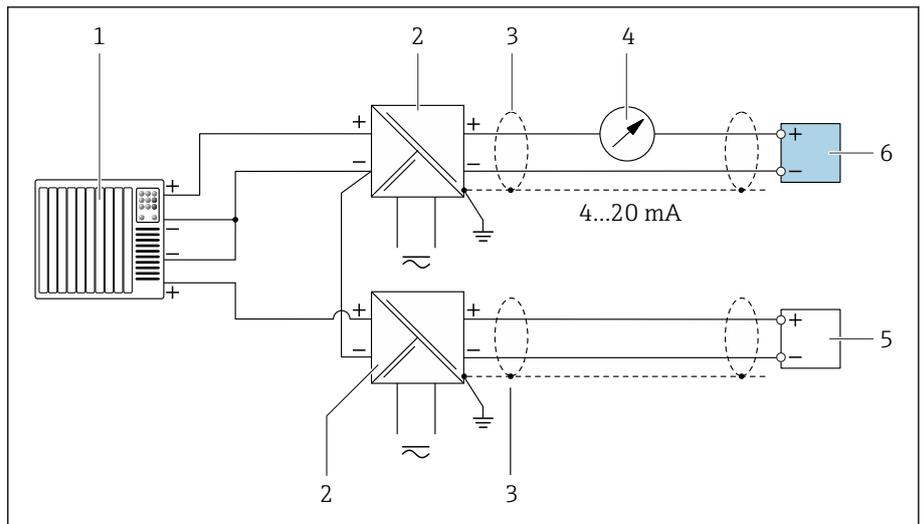


A0028763

1 Connection example for HART input with a common negative (passive)

- 1 Automation system with current input, e.g. PLC
- 2 Active barrier for supply voltage, e.g. RN221N
- 3 Cable shield
- 4 Analog display unit: observe max. load.
- 5 Pressure measuring device, e.g. Cerabar M, Cerabar S: observe requirements
- 6 Transmitter

Modbus RS485

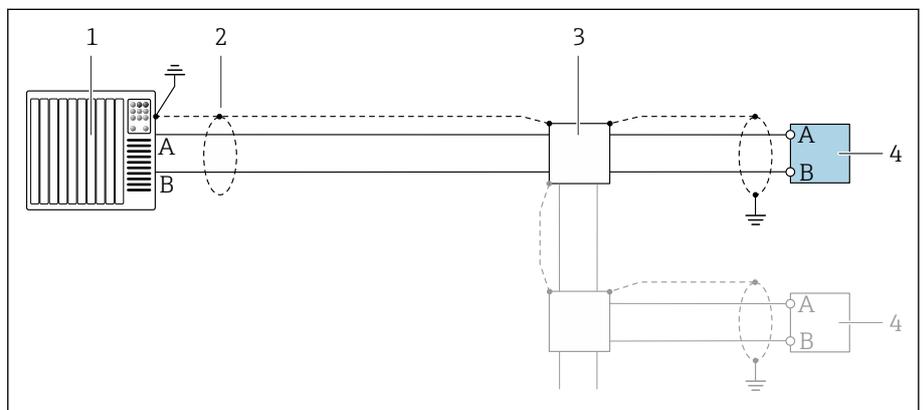


A0028765

2 Connection example for Modbus RS485, non-hazardous area and Zone 2; Class I, Division 2

- 1 Automation system, e.g. PLC
- 2 Cable shield
- 3 Distribution box
- 4 Transmitter


Current output 4 to 20 mA (active)

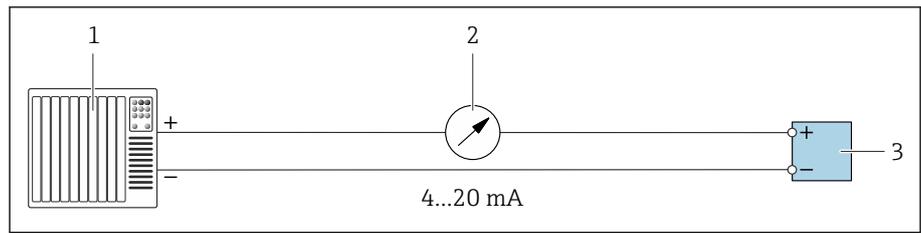

A0028758

- 1 Automation system with current input, e.g. PLC
- 2 Analog display unit: observe max. load.
- 3 Transmitter


Current output 4 to 20 mA (passive)

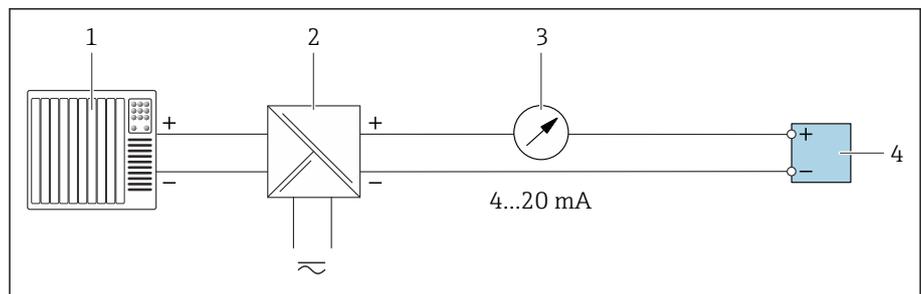

A0028759

- 1 Automation system with current input, e.g. PLC
- 2 Active barrier for supply voltage, e.g. RN221N
- 3 Analog display unit: observe max. load.
- 4 Transmitter


Pulse/frequency output (passive)

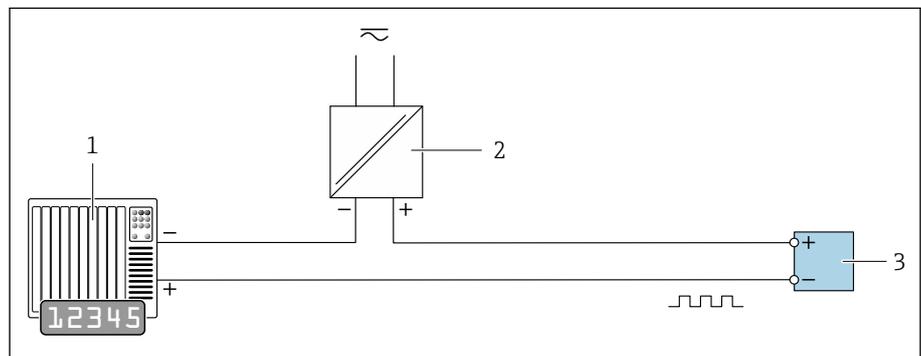

A0028761

- 1 Automation system with pulse output and frequency input, e.g. PLC
- 2 Supply voltage
- 3 Transmitter: observe input values.

Switch output (passive)

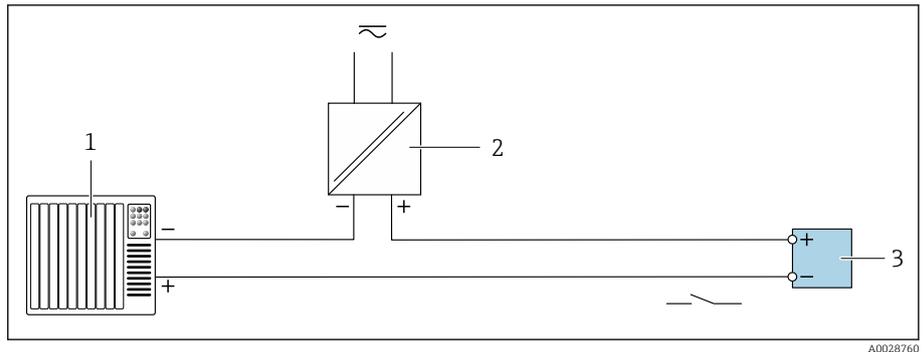

- 1 Automation system with switch input, e.g. PLC
- 2 Supply voltage
- 3 Transmitter: observe input values.

Potential equalization

Metal process connections


Potential equalization is via the metal process connections that are in contact with the medium and mounted directly on the sensor.

Plastic process connections

Note the following when using grounding rings:

- Depending on the option ordered, plastic disks are used instead of grounding rings on some process connections. The plastic disks act as "spacers" and do not have any potential equalization function. They perform a significant sealing function at the sensor and process connection interfaces. In the case of process connections without metal grounding rings, the plastic disks and seals must never be removed. Plastic disks and seals must always be installed.
- Grounding rings can be ordered separately as an accessory from Endress+Hauser. The grounding rings must be compatible with the electrode material, as otherwise there is the danger that the electrodes could be destroyed by electrochemical corrosion.
- Grounding rings, including seals, are installed inside the process connections. This does not affect the installation length.

Connection example for potential equalization with additional grounding ring

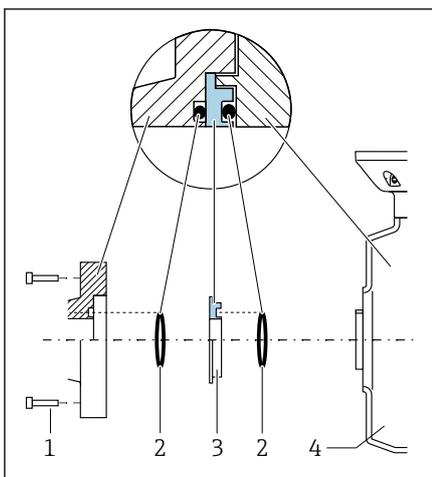

**NOTICE**


**If potential equalization is not provided, this can lead to the electrochemical degradation of the electrodes or affect measuring accuracy!**

Damage to the device.

- ▶ Install grounding rings.
- ▶ Provide (establish) potential equalization.

1. Loosen the hexagonal-headed bolts (1).
2. Remove the process connection from the sensor (4).
3. Remove the plastic disk (3), along with the seals (2), from the process connection.
4. Place the first seal (2) into the groove of the process connection.
5. Place the metal grounding ring (3) into the process connection.
6. Place the second seal (2) into the groove of the grounding ring.
7. Observe the maximum screw tightening torques for lubricated threads: 7 Nm (5.2 lbf ft)
8. Mount the process connection on the sensor (4).

Connection example for potential equalization with grounding electrodes

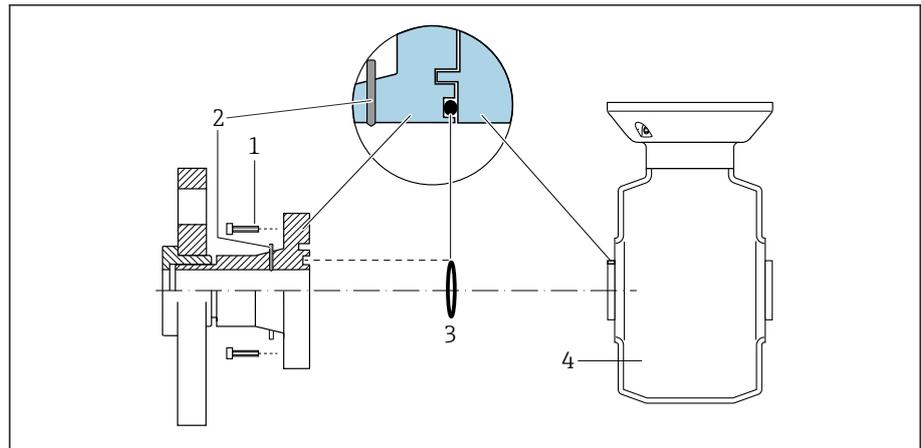

A0028972

- 1 Hexagonal-headed bolts of process connection
- 2 Integrated grounding electrodes
- 3 Seal
- 4 Sensor

### Terminals

#### Spring terminals

- Suitable for strands and strands with ferrules.
- Conductor cross-section 0.2 to 2.5 mm<sup>2</sup> (24 to 12 AWG).

### Cable entries

- Cable gland: M20 × 1.5 for cable Ø6 to 12 mm (0.24 to 0.47 in)
- Thread for cable entry:
  - NPT ½"
  - G ½", G ½" Ex d
  - M20

## Cable specification

---

Requirements for connecting cable	30
Ground cable requirements	30
Connecting cable requirements	30

## Requirements for connecting cable

### Electrical safety

As per applicable national regulations.

### Permitted temperature range

- Observe the installation guidelines that apply in the country of installation.
- The cables must be suitable for the minimum temperatures and maximum temperatures to be expected.

### Power supply cable (incl. conductor for the inner ground terminal)

- A standard installation cable is sufficient.
- Provide grounding according to applicable national codes and regulations.


### Signal cable

- Current output 4 to 20 mA HART:  
A shielded cable is recommended, observe the grounding concept of the facility.
- Pulse/frequency/switch output:  
Standard installation cable
- Modbus RS485:  
Cable type A according to EIA/TIA-485 standard is recommended
- Current output 4 to 20 mA:  
Standard installation cable

### Ground cable requirements

Copper wire: at least 6 mm<sup>2</sup> (0.0093 in<sup>2</sup>)

### Connecting cable requirements

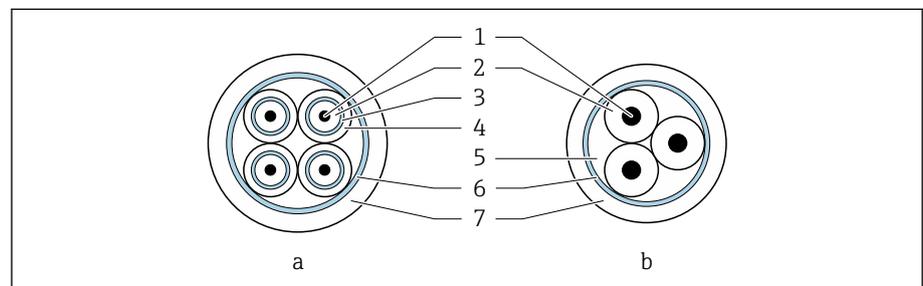

A0029151

3 Cable cross-section

- a* Electrode cable
- b* Coil current cable
- 1 Core
- 2 Core insulation
- 3 Core shield
- 4 Core jacket
- 5 Core reinforcement
- 6 Cable shield
- 7 Outer jacket

## Electrode cable

<b>Design</b>	3×0.38 mm <sup>2</sup> (20 AWG) with common, braided copper shield (∅ ~ 9.5 mm (0.37 in)) and individual shielded cores If using the empty pipe detection (EPD) function: 4×0.38 mm <sup>2</sup> (20 AWG) with common, braided copper shield (∅ ~ 9.5 mm (0.37 in)) and individual shielded cores
<b>Conductor resistance</b>	≤ 50 Ω/km (0.015 Ω/ft)
<b>Capacitance: core/shield</b>	≤ 420 pF/m (128 pF/ft)
<b>Cable length</b>	Depending on the medium conductivity: maximum 200 m (656 ft)
<b>Cable lengths (available for order)</b>	5 m (15 ft), 10 m (30 ft), 20 m (60 ft) or variable length: maximum 200 m (656 ft)
<b>Operating temperature</b>	-20 to +80 °C (-4 to +176 °F)

## Coil current cable

<b>Design</b>	3×0.38 mm <sup>2</sup> (20 AWG) with common, braided copper shield (∅ ~ 9.5 mm (0.37 in)) and individual shielded cores
<b>Conductor resistance</b>	≤ 37 Ω/km (0.011 Ω/ft)
<b>Capacitance: core/shield</b>	≤ 120 pF/m (37 pF/ft)
<b>Cable length</b>	Depends on the medium conductivity, max. 200 m (656 ft)
<b>Cable lengths (available for order)</b>	5 m (15 ft), 10 m (30 ft), 20 m (60 ft) or variable length up to max. 200 m (656 ft)
<b>Operating temperature</b>	-20 to +80 °C (-4 to +176 °F)
<b>Test voltage for cable insulation</b>	≤ AC 1 433 V r.m.s. 50/60 Hz or ≥ DC 2 026 V

---

## Performance characteristics

---

Reference operating conditions	34
Maximum measured error	34
Repeatability	34
Temperature measurement response time	35
Influence of ambient temperature	35

### Reference operating conditions

- Error limits based on ISO 20456:2017
- Water, typically: +15 to +45 °C (+59 to +113 °F); 0.5 to 7 bar (7.3 to 101 psi)
- Data as indicated in the calibration protocol
- Accuracy based on accredited calibration rigs according to ISO 17025
- Reference temperature for conductivity measurement: 25 °C (77 °F)

**i** To obtain measured errors, use the *Applicator* sizing tool → *Service-specific accessory*, 101

### Maximum measured error


o. r. = of reading

### Error limits under reference operating conditions

#### Volume flow

±0.5 % o. r. ±1 mm/s (±0.04 in/s)

**i** Fluctuations in the supply voltage do not have any effect within the specified range.

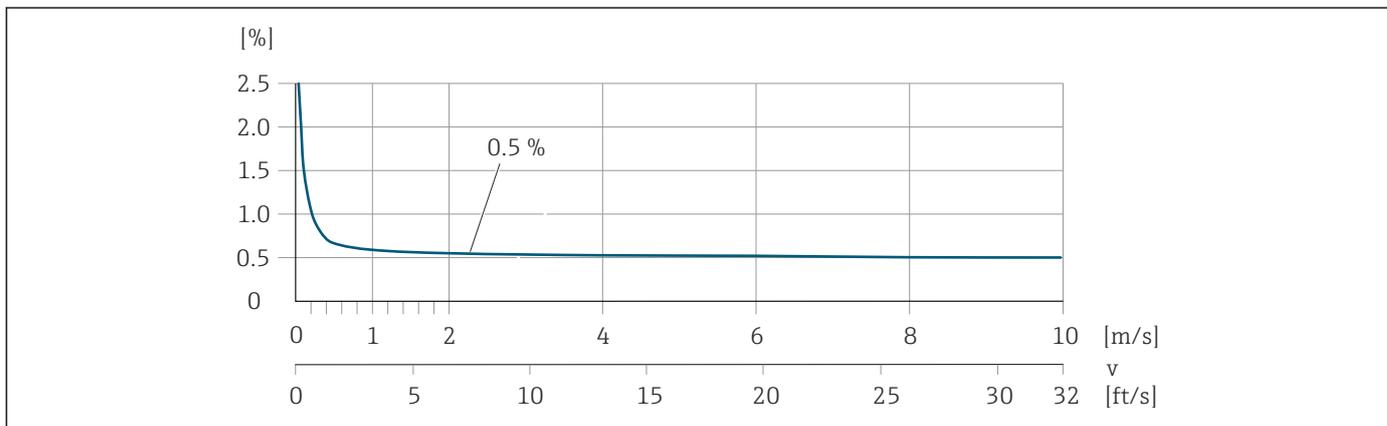

A0045827

#### Temperature

±3 °C (±5.4 °F)

#### Electrical conductivity

Max. measured error not specified.

### Accuracy of outputs

Current output	±5 µA
Pulse/frequency output	Max. ±100 ppm o. r. (across the entire ambient temperature range)

### Repeatability

Volume flow	Max. ±0.1 % o. r. ± 0.5 mm/s (0.02 in/s)
Electrical conductivity	<ul style="list-style-type: none"> <li>▪ Max. ±5 % o. r. (5 to 100 000 µS/cm)</li> <li>▪ Max. ±1 % o. r. for DN 15 to 150 in conjunction with stainless steel process connections, 1.4404 (F316L)</li> </ul>
Temperature	±0.5 °C (±0.9 °F)

### Temperature measurement response time

$T_{90} < 15 \text{ s}$

### Influence of ambient temperature

<b>Current output</b>	Temperature coefficient max. $1 \mu\text{A}/^\circ\text{C}$
<b>Pulse/frequency output</b>	No additional effect. Is included in the accuracy.

---


# Installation

---

Installation conditions

## Installation conditions

### Flow direction

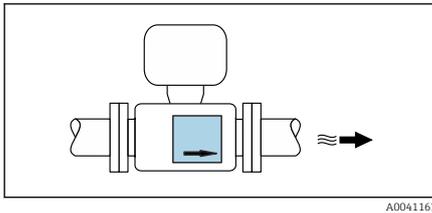


A0041163

Install the device in the direction of flow.



Note the direction of arrow on the nameplate.

### Inlet runs and outlet runs

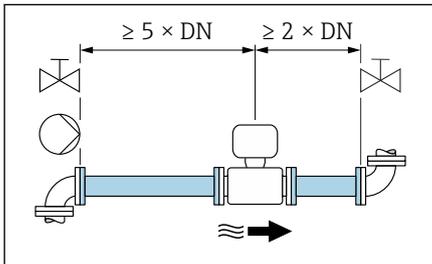


A0028997

Ensure straight, undisturbed inlet and outlet runs.




To avoid negative pressure and to comply with accuracy specifications, install the sensor upstream from assemblies that produce turbulence (e.g. valves, T-sections) and downstream from pumps → *Installation near pumps*, 40.

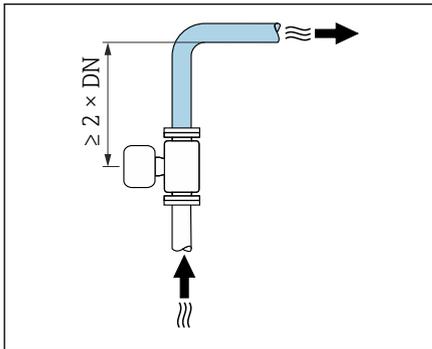

A0042132


Keep a sufficient distance to the next pipe elbow.

### Orientations

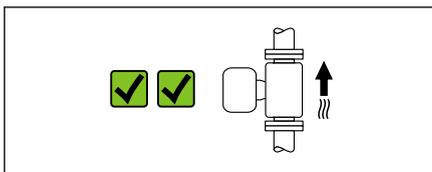

A0041159

**Vertical orientation, upward direction of flow**  
For all applications.

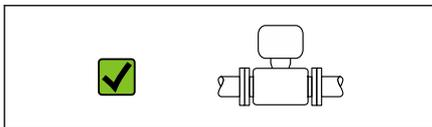


A0041160

**Horizontal orientation, transmitter at top**

This orientation is suitable for the following applications:


- For low process temperatures in order to maintain the minimum ambient temperature for the transmitter.
- For empty pipe detection, even in the case of empty or partially filled measuring pipes.

### Mounting locations

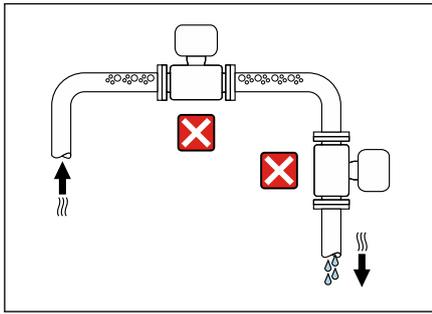


- Do not install the device at the highest point of the pipe.
- Do not install the device upstream from a free pipe outlet in a down pipe.

A0042131

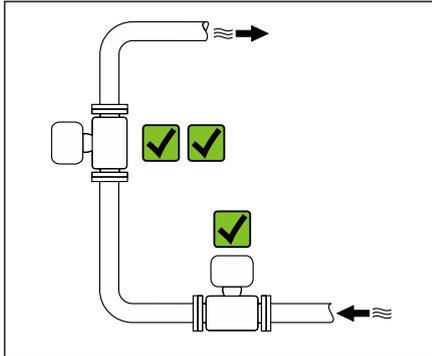

A0042317


### Installation near control valves

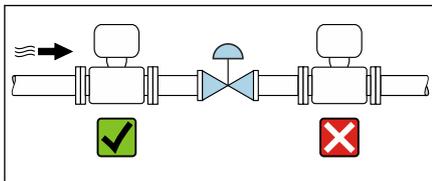

Install the device in the direction of flow upstream from the control valve.

A0041091

### Installation upstream from a down pipe

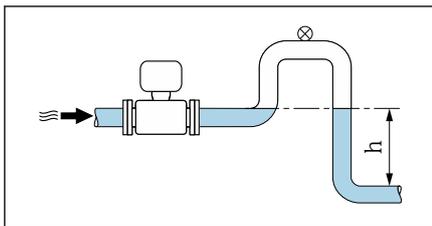

A0041089


#### NOTICE

**Negative pressure in the measuring pipe can damage the liner!**

- ▶ If installing upstream from down pipes with a length  $h \geq 5 \text{ m}$  (16.4 ft): install a siphon with a vent valve downstream from the device.

**i** This arrangement prevents the flow of liquid stopping in the pipe and air entrainment.

### Installation with partially filled pipes

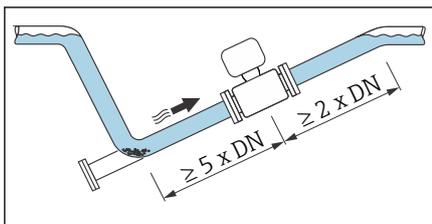

A0041088


- Partially filled pipes with a gradient require a drain-type configuration.
- The installation of a cleaning valve is recommended.

### Installation near pumps

#### NOTICE

**Negative pressure in the measuring pipe can damage the liner!**

- ▶ Install the device in the direction of flow downstream from the pump.
- ▶ Install pulsation dampers if reciprocating, diaphragm or peristaltic pumps are used.

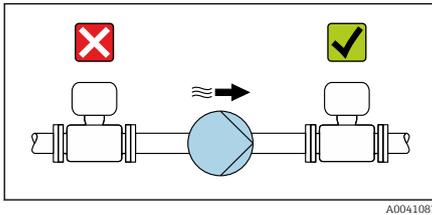


### Pipe vibrations

A remote version is recommended in the event of strong pipe vibrations.


#### NOTICE

**Pipe vibrations can damage the device!**

- ▶ Do not expose the device to strong vibrations.
- ▶ Support the pipe and fix it in place.
- ▶ Support the device and fix it in place.
- ▶ Mount the sensor and transmitter separately.

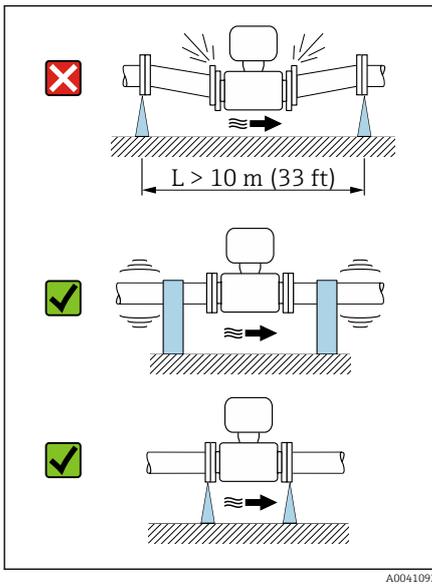

### Adapters

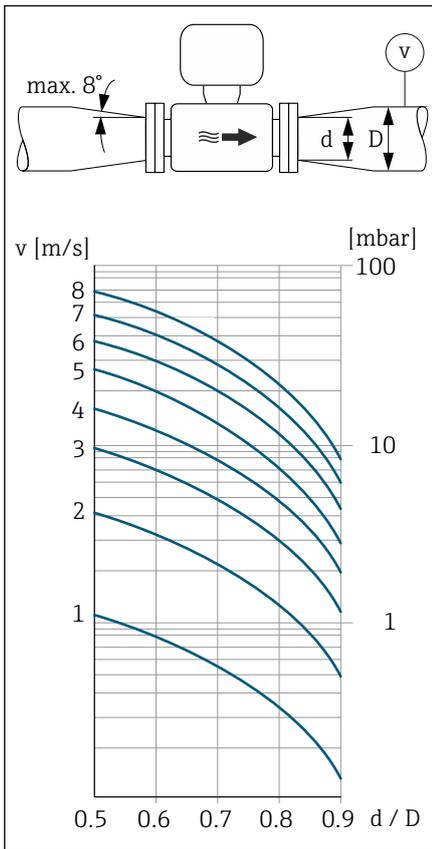

Suitable adapters (double-flange reducers) can be used to install the sensor in larger-diameter pipes. The resulting higher rate of flow improves measuring accuracy with very slow-moving media.

**i** The nomogram shown here can be used to calculate the pressure loss caused by reducers and expanders. It only applies to liquids with a viscosity similar to that of water.


1. Calculate the ratio of the diameters  $d/D$ .
2. Determine the flow velocity after the reduction.
3. From the chart, determine the pressure loss as a function of the flow velocity  $v$  and the  $d/D$  ratio.

### Seals


Note the following when installing seals:  
For plastic flanges: seals are **always** required.

### Magnetism and static electricity

Do not install the device near magnetic fields, e.g. motors, pumps, transformers.

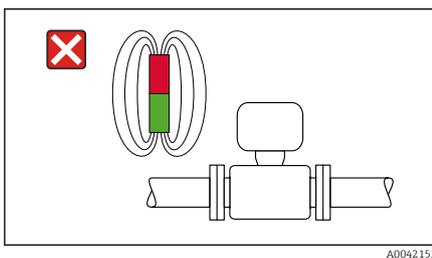

### Outdoor use

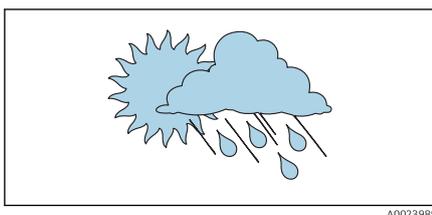

- Avoid exposure to direct sunlight.
- Install in a location protected from sunlight.
- Avoid direct exposure to weather conditions.
- Use a weather protection cover → *Transmitter*, 100.

---

## Environment

---

Ambient temperature range	44
Storage temperature	44
Degree of protection	44
Vibration-resistance and shock-resistance	44
Interior cleaning	45
Electromagnetic compatibility (EMC)	45

### Ambient temperature range

<b>Transmitter</b>	-40 to +60 °C (-40 to +140 °F)
<b>Local display</b>	-20 to +60 °C (-4 to +140 °F) The readability of the display may be impaired at temperatures outside the temperature range.
<b>Sensor</b>	-40 to +60 °C (-40 to +140 °F)
<b>Liner</b>	Do not exceed or fall below the permitted temperature range of the liner .  Dependency of ambient temperature on medium temperature → <i>Medium temperature range</i> ,  48

### Storage temperature

The storage temperature corresponds to the ambient temperature range of the transmitter and sensor.

### Degree of protection

<b>Transmitter</b>	<ul style="list-style-type: none"> <li>■ IP66/67, type 4X enclosure</li> <li>■ Open housing: IP20, type 1 enclosure</li> </ul>
<b>Sensor</b>	IP66/67, type 4X enclosure

### Vibration-resistance and shock-resistance

#### Compact version

<b>Vibration, sinusoidal</b> <ul style="list-style-type: none"> <li>■ Following IEC 60068-2-6</li> <li>■ 20 cycles per axis</li> </ul>	2 to 8.4 Hz	3.5 mm peak
	8.4 to 2 000 Hz	1 g peak
<b>Vibration, broad-band random</b> <ul style="list-style-type: none"> <li>■ Following IEC 60068-2-64</li> <li>■ 120 min per axis</li> </ul>	10 to 200 Hz	0.003 g <sup>2</sup> /Hz
	200 to 2 000 Hz	0.001 g <sup>2</sup> /Hz (1.54 g rms)
<b>Shocks, half-sine</b> <ul style="list-style-type: none"> <li>■ Following IEC 60068-2-27</li> <li>■ 3 positive and 3 negative shocks</li> </ul>	6 ms 30 g	

#### Shock

Due to rough handling according to IEC 60068-2-31.

#### Remote version (sensor)

<b>Vibration, sinusoidal</b> <ul style="list-style-type: none"> <li>■ Following IEC 60068-2-6</li> <li>■ 20 cycles per axis</li> </ul>	2 to 8.4 Hz	7.5 mm peak
	8.4 to 2 000 Hz	2 g peak
<b>Vibration, broad-band random</b> <ul style="list-style-type: none"> <li>■ Following IEC 60068-2-6</li> <li>■ 120 min per axis</li> </ul>	10 to 200 Hz	0.01 g <sup>2</sup> /Hz
	200 to 2 000 Hz	0.003 g <sup>2</sup> /Hz (2.7 g rms)
<b>Shocks, half-sine</b> <ul style="list-style-type: none"> <li>■ Following IEC 60068-2-6</li> <li>■ 3 positive and 3 negative shocks</li> </ul>	6 ms 50 g	

#### Shock

Due to rough handling according to IEC 60068-2-31.

### Interior cleaning

Available methods of internal cleaning:

- Cleaning in place (CIP)
- Sterilization in place (SIP)

### Electromagnetic compatibility (EMC)

As per IEC/EN 61326 and NAMUR Recommendation NE 21.



For more information: Declaration of Conformity

---


## Process

---

Medium temperature range	48
Conductivity	48
Flow limit	48
Pressure-temperature ratings	50
Pressure tightness	52
Pressure loss	52

### Medium temperature range

-20 to +150 °C (-4 to +302 °F)

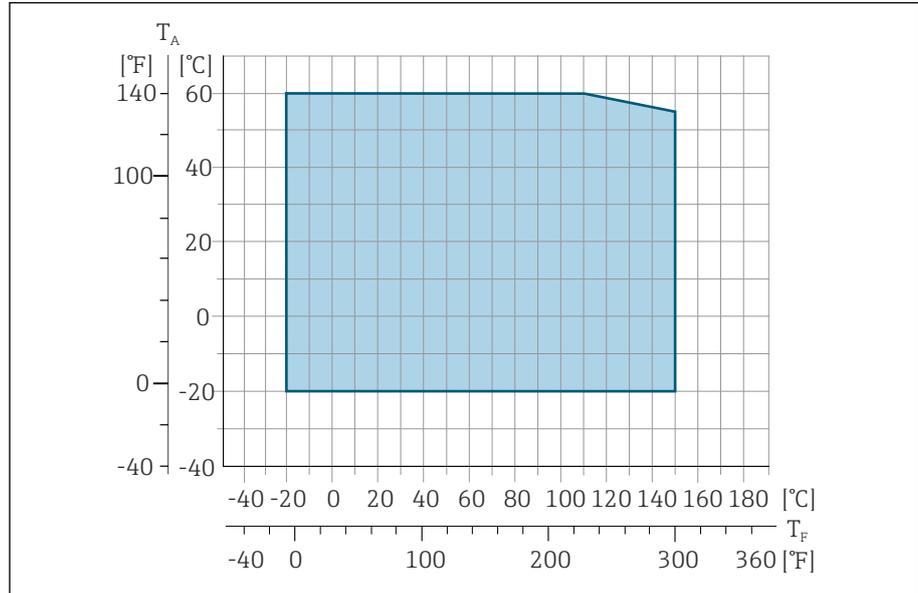


A0027450

$T_A$  Ambient temperature  
 $T_F$  Medium temperature

### Conductivity

The necessary minimum conductivity is  $\geq 5 \mu\text{S/cm}$ .

**i** Note that in the case of the remote version, the minimum conductivity depends on the cable length.

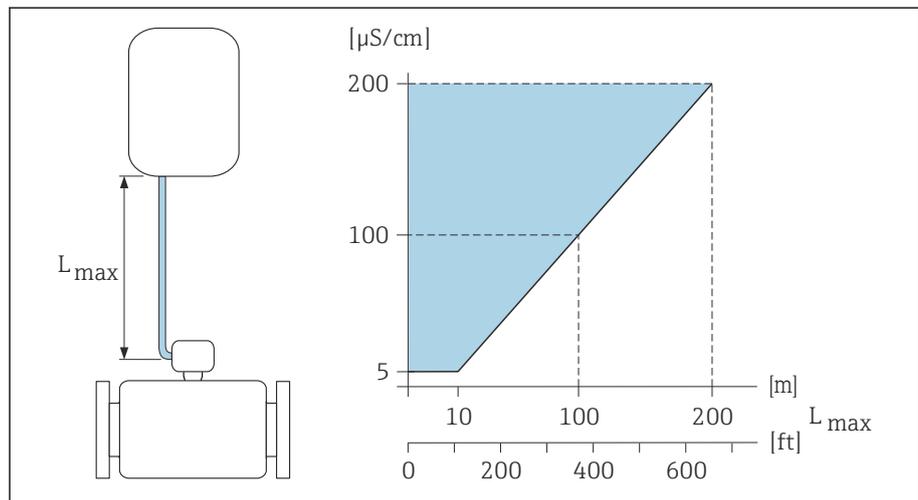

A0016539

**4** Permitted length of connecting cable

Colored area = permitted range  
 $L_{\text{max}}$  = length of connecting cable in [m] ([ft])  
 $[\mu\text{S/cm}]$  = medium conductivity

### Flow limit

Pipe diameter and flow rate determine the nominal diameter of the sensor.

**i** The flow velocity is increased by reducing the sensor nominal diameter.

2 to 3 m/s (6.56 to 9.84 ft/s)	Optimum flow velocity
$v < 2$ m/s (6.56 ft/s)	For low conductivity values
$v > 2$ m/s (6.56 ft/s)	For media producing buildup, e.g. high-fat milk

### Pressure-temperature ratings


Maximum permitted medium pressure as a function of the medium temperature.  
The data relate to all pressure bearing parts of the device.

### Process connections with O-ring seal, DN 2 to 25 (1/12 to 1")

Maximum permitted medium pressure as a function of the medium temperature.  
The data relate to all pressure bearing parts of the device.

#### Fixed flange according to EN 1092-1


Stainless steel

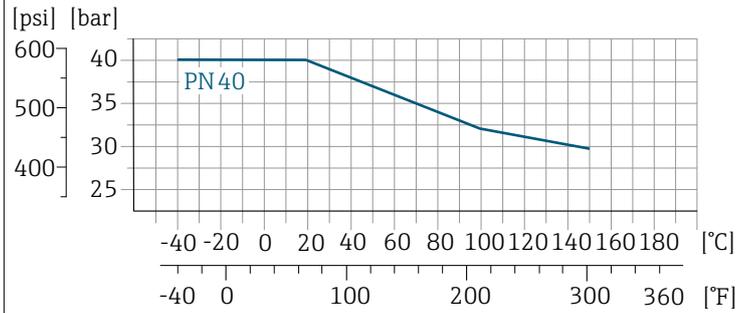

A0028928-EN

#### Fixed flange according to ASME B16.5


Stainless steel

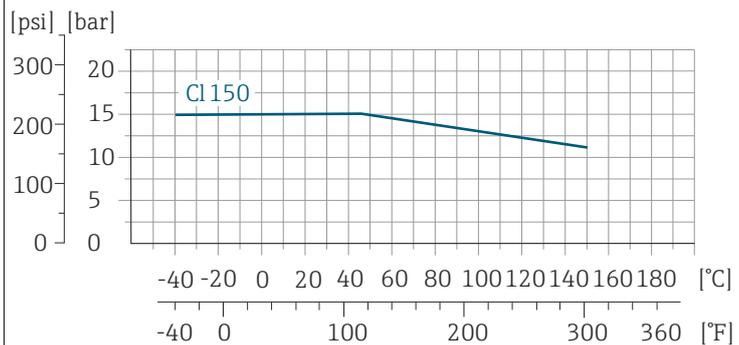

A0028936-EN

#### Fixed flange according to JIS B2220


Stainless steel

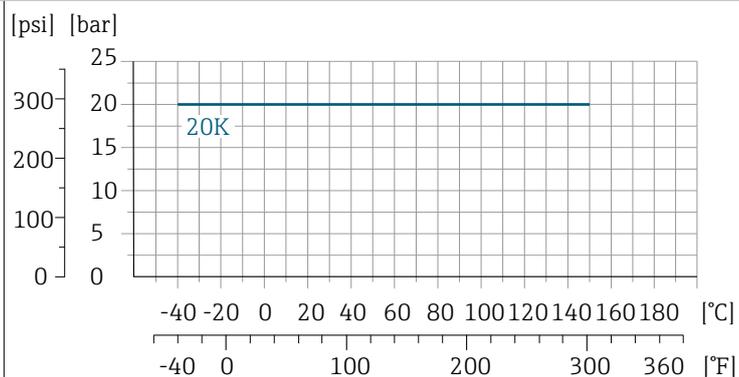

A0028938-EN

**Thread according to ISO 228  
Welding socket according to ISO 2037**

Stainless steel

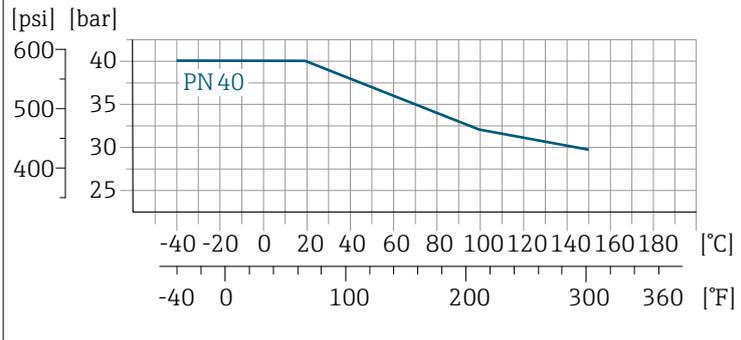


A0028928-EN

Process connections with aseptic gasket seal, DN 2 to 25 (1/12 to 1")

**Welding socket according to EN 10357 (DIN 11850)  
Thread according to DIN 11851 SC  
Thread according to DIN 11864-1  
Flange DIN 11864-2 Form**

Stainless steel

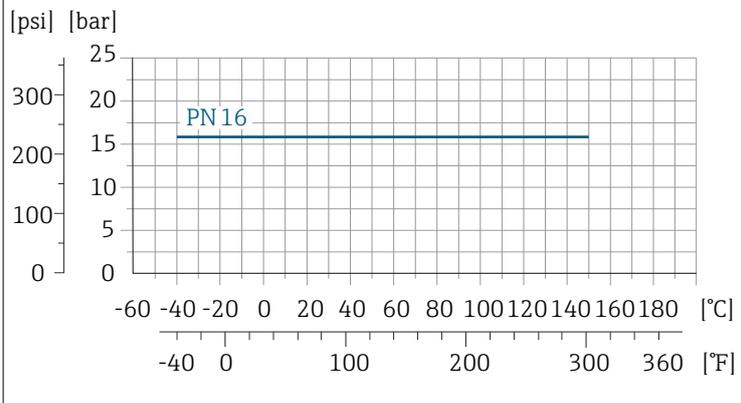


A0028940-EN

Process connections with aseptic gasket seal, DN 40 to 150 (1 1/2 to 6")

**Welding socket according to ASME BPE A0028942-DE  
Welding socket according to EN 10357 (DIN 11850)  
Welding socket according to ISO 2037  
Thread according to DIN 11851 SC**


Stainless steel

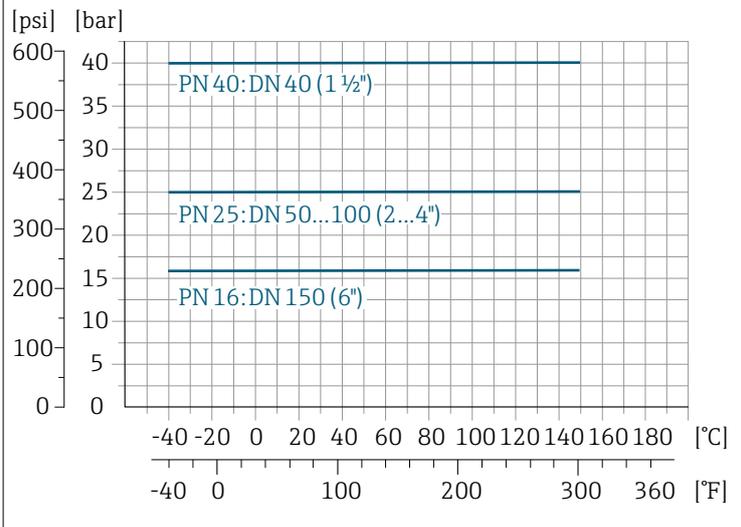

A0028942-EN

**Flange DIN 11864-2 Form A, flange with notch**  
**Thread according to DIN 11864-1**

Stainless steel

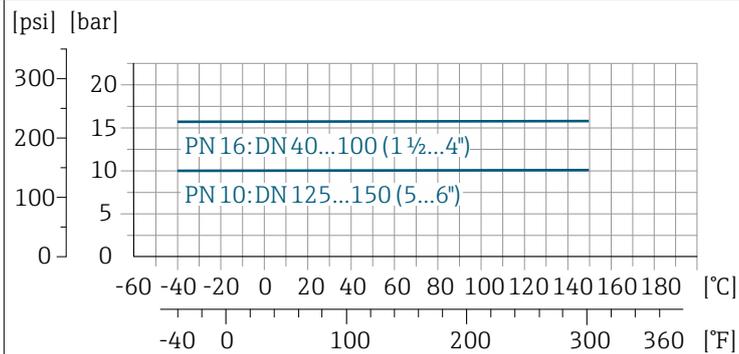

A0028943-EN

**Tri-clamp**

Stainless steel

The clamp connections are suitable up to a maximum pressure of 16 bar (232 psi). Please observe the operating limits of the clamp and seal used as they can be over 16 bar (232 psi). The clamp and seal are not included in the scope of supply.

**Pressure tightness**

Limit values for the absolute pressure depending on the liner and medium temperature

PFA	Nominal diameter		Absolute pressure in [mbar] ([psi])				
	[mm]	[in]	+25 °C (+77 °F)	+80 °C (+176 °F)	+100 °C (+212 °F)	+130 °C (+266 °F)	+150 °C (+302 °F)
	2 to 150	1/12 to 6	0 (0)	0 (0)	0 (0)	0 (0)	0 (0)

**Pressure loss**

- No pressure loss: as of DN 8 (5/16"), with transmitter installed in a pipe with the same nominal diameter.
- Pressure loss information when adapters are used → *Adapters*, 41

## Mechanical construction

---

Weight	54
Measuring pipe specification	54
Materials	55
Fitted electrodes	56
Surface roughness	56

## Weight

All values refer to devices with flanges with a standard pressure rating.  
Weight data are guideline values. The weight may be lower than indicated depending on the pressure rating and design.

### Transmitter remote version

Aluminum: 2.4 kg (5.3 lbs)

### Sensor remote version

Aluminum sensor connection housing: see the information in the following table.

Nominal diameter		Weight	
[mm]	[in]	[kg]	[lbs]
2	1/12	4.7	10.4
4	5/32	4.7	10.4
8	5/16	4.7	10.4
15	½	4.6	10.1
25	1	5.5	12.1
40	1 ½	6.8	15.0
50	2	7.3	16.1
65	–	8.1	17.9
80	3	8.7	19.2
100	4	10.0	22.1
125	5	15.4	34.0
150	6	17.8	39.3

## Measuring pipe specification

Nominal diameter		Pressure rating <sup>1)</sup> EN (DIN) [bar]	Process connection internal diameter	
[mm]	[in]		PFA	
[mm]	[in]	[bar]	[mm]	[in]
2	1/12	PN 16/40	2.25	0.09
4	5/32	PN 16/40	4.5	0.18
8	5/16	PN 16/40	9.0	0.35
15	½	PN 16/40	16.0	0.63
–	1	PN 16/40	22.6	0.89
25	–	PN 16/40	26.0	1.02
40	1 ½	PN 16/25/40	35.3	1.39
50	2	PN 16/25	48.1	1.89
65	–	PN 16/25	59.9	2.36
80	3	PN 16/25	72.6	2.86
100	4	PN 16/25	97.5	3.84
125	5	PN 10/16	120.0	4.72
150	6	PN 10/16	146.5	5.77

1) Depending on process connection and seals used

## Materials

<b>Transmitter housing</b>	
Order code for "Housing"	Option A: aluminum, AlSi10Mg, coated
Window material	Glass
<b>Sensor connection housing</b>	
	Stainless steel 1.4301 (304)
<b>Cable glands and entries</b>	
Cable gland M20×1.5	Plastic
Adapter for cable entry with female thread G ½" or NPT ½"	Nickel-plated brass
<b>Connecting cable for remote version</b>	
	Electrode and coil current cable: PVC cable with copper shield
<b>Sensor housing</b>	
	Stainless steel: 1.4301 (304)
<b>Measuring pipes</b>	
	Stainless steel: 1.4301 (304)
<b>Liner</b>	
	PFA (USP Class VI, FDA 21 CFR 177.2600)
<b>Electrodes</b>	
	Stainless steel: 1.4435 (316L)
<b>Seals</b>	
	<ul style="list-style-type: none"> <li>■ O-ring seal, DN 2 to 25 (1/12 to 1"): EPDM, FKM, Kalrez</li> <li>■ Aseptic (hygienic design) gasket seal, DN 2 to 150 (1/12 to 6"): EPDM, FKM, VMQ (silicone)</li> </ul>
<b>Process connections</b>	
	<ul style="list-style-type: none"> <li>■ Stainless steel, 1.4404 (F316L)</li> <li>■ PVDF</li> <li>■ PVC adhesive sleeve</li> </ul>
<b>Wall mounting kit</b>	
	Stainless steel 1.4301 (304) Does not meet the hygienic design installation guidelines.
<b>Spacer</b>	
	Stainless steel 1.4435 (F316L)

**Accessories**

Protective cover	Stainless steel, 1.4404 (316L)
Pipe mounting set	Stainless steel 1.4301 (304)
Wall mounting kit	Stainless steel 1.4301 (304) Does not meet the hygienic design installation guidelines.

**Fitted electrodes**

Standard electrodes:

- Measuring electrodes
- Empty pipe detection electrode (only DN 15 to 150 (½ to 6"))

**Surface roughness**

Data relate to surfaces in contact with the medium.

Stainless steel electrodes, 1.4435 (316L); Alloy C22, 2.4602 (UNS N06022); platinum;  
tantalum:

≤ 0.3 to 0.5 μm (11.8 to 19.7 μin)

Liner with PFA:

≤ 0.4 μm (15.7 μin)

Stainless steel process connections:

- With O-ring seal: Ra ≤ 1.6 μm (63 μin)
- With aseptic seal: R<sub>amax</sub> = 0.76 μm (30 μin),


## Dimensions in SI units

---

<b>Compact version</b>	<b>58</b>
Order code for "Housing", option A "Aluminum, coated"	58
<b>Remote version</b>	<b>59</b>
Transmitter remote version	59
Sensor remote version	60
<b>Sensor flange connection</b>	<b>61</b>
<b>Flange connections</b>	<b>63</b>
Flange DIN 11864-2 Form A, female	63
Flange DIN 11864-2 Form A, flange with notch	63
Flange in accordance with EN 1092-1 (DIN 2501 / DIN 2512N): PN 40	64
Flange according to ASME B16.5, Class 150	64
Flange according to JIS B2220, 20K	65
<b>Clamp connections</b>	<b>66</b>
Tri-Clamp	66
<b>Welding socket</b>	<b>67</b>
Welding socket according to EN 10357	67
Welding socket according to ISO 2037	67
Welding socket according to ASME BPE	68
<b>Couplings</b>	<b>69</b>
Thread according to DIN 11851 SC	69
Thread according to DIN 11864-1, Form A	70
Male thread according to ISO 228/DIN 2999	71
<b>Mounting kit</b>	<b>72</b>
Wall mounting kit	72
<b>Accessories</b>	<b>73</b>
Grounding rings	73
Spacer	73
Male thread with O-ring seal	74
Female thread with O-ring seal	74
Tri-Clamp	75
Protective cover	75

## Compact version

Order code for "Housing", option A "Aluminum, coated"

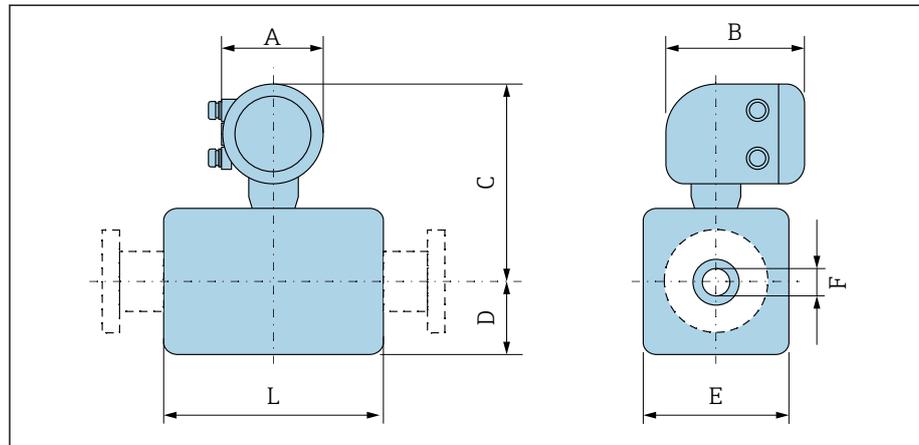

A0043172


DN		A <sup>1)</sup>	B	C	D	E	F	L <sup>2)</sup>
[mm]	[in]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
2	1/12	139	178	235	48	43	2.25	86
4	1/32	139	178	235	48	43	4.5	86
8	5/16	139	178	235	48	43	9	86
15	1/2	139	178	235	48	43	16	86
-	1	139	178	239	52	56	22.6	86
25	-	139	178	239	52	56	26.0	86
40	1 1/2	139	178	242	54	107	34.8	140
50	2	139	178	249	60	120	47.5	140
65	-	139	178	256	68	135	60.2	140
80	3	139	178	263	74	148	72.9	140
100	4	139	178	276	87	174	97.4	140
125	-	139	178	292	103	206	120.0	200
150	6	139	178	306	117	234	146.9	200

1) Depending on the cable gland used: values up to + 30 mm

2) Total length depends on the process connections.

### Remote version

#### Transmitter remote version

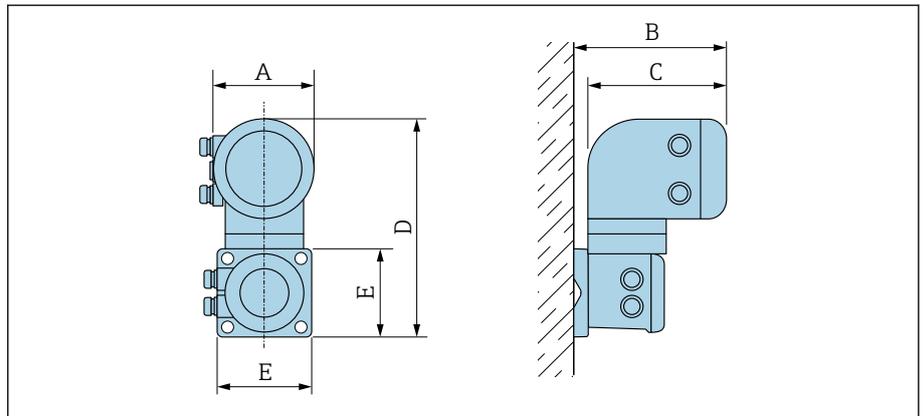


A0042715

Order code for "Housing"	A <sup>1)</sup> [mm]	B [mm]	C [mm]	D [mm]	E [mm]
Option P "Remote, aluminum, coated"	139	185	178	309	130

1) Depending on the cable entry used: values up to + 30 mm

## Sensor remote version

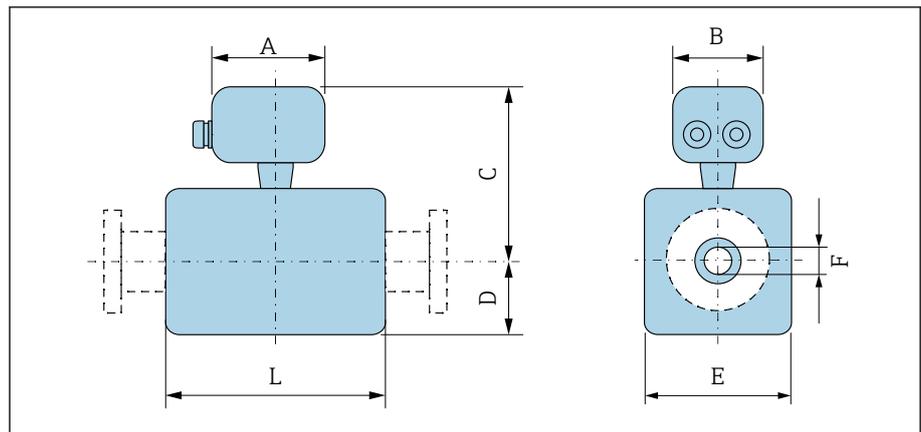


A0043178

DN		A <sup>1)</sup>	B	C	D	E	F	L <sup>2)</sup>
[mm]	[in]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
2	1/12	183	207	129	55	43	2.25	86
4	1/32	183	207	129	55	43	4.5	86
8	5/16	183	207	129	55	43	9	86
15	1/2	183	207	129	55	43	16	86
-	1	183	207	133	55	56	22.6	86
25	-	183	207	133	55	56	26.0	86
40	1 1/2	183	207	136	54	107	34.8	140
50	2	183	207	143	60	120	47.5	140
65	-	183	207	150	67	135	60.2	140
80	3	183	207	157	74	148	72.9	140
100	4	183	207	170	87	174	97.4	140
125	-	183	207	186	103	206	120.0	200
150	6	183	207	200	117	234	146.9	200

1) Depending on the cable gland used: values up to + 30 mm

2) Total length depends on the process connections.


Sensor flange connection

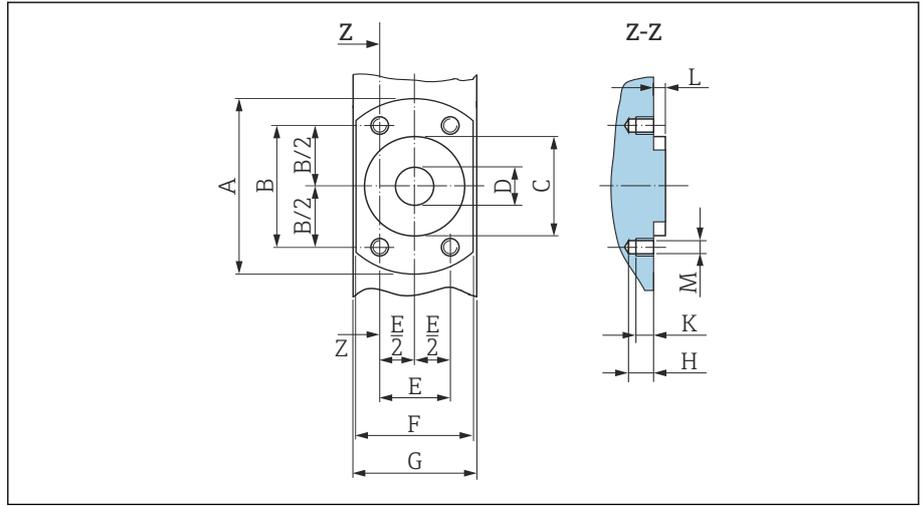

A0017657

5 Front view without process connections

DN		A	B	C	D	E	F	G	H	K	L	M
[mm]	[in]	[mm]										
2	1/12	62	41.6	34	9	24	42	43	8.5	6	4	M6
4	1/32	62	41.6	34	9	24	42	43	8.5	6	4	M6
8	5/16	62	41.6	34	9	24	42	43	8.5	6	4	M6
15	1/2	62	41.6	34	16	24	42	43	8.5	6	4	M6
25	-	72	50.2	44	26	29	55	56	8.5	6	4	M6

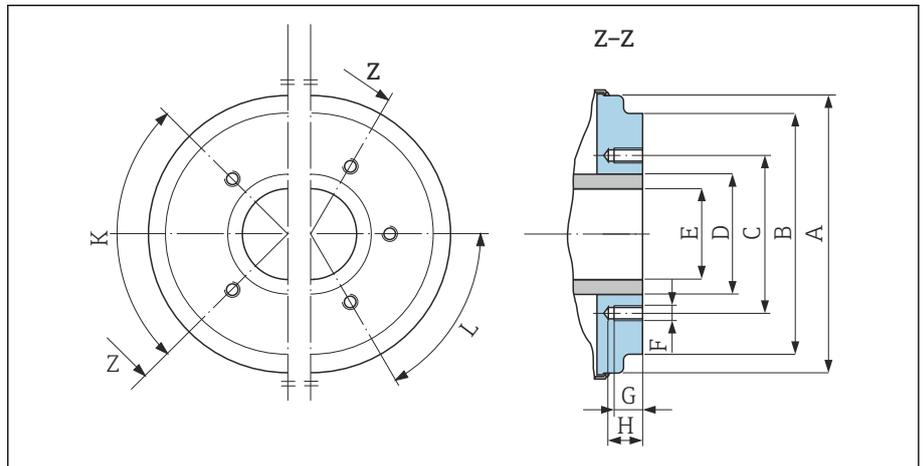

A0005528

6 Front view without process connections

DN		A	B	C	D	E	F	G	H	K	L
[mm]	[in]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	90° ±0.5°	60° ±0.5°
											Tapped holes
40	1 1/2	99.7	85.8	71.0	48.3	34.8	M8	12	17	4	-
50	2	112.7	98.8	83.5	60.3	47.5	M8	12	17	4	-
65	-	127.7	114.8	100.0	76.1	60.2	M8	12	17	-	6
80	3	140.7	133.5	114.0	88.9	72.9	M8	12	17	-	6

DN		A	B	C	D	E	F	G	H	K	L
[mm]	[in]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	[mm]	90° ±0.5°	60° ±0.5°
		Tapped holes									
100	4	166.7	159.5	141.0	114.3	97.4	M8	12	17	-	6
125	-	198.7	191.5	171.0	139.7	120.0	M10	15	20	-	6
150	6	226.7	219.5	200.0	168.3	146.9	M10	15	20	-	6

### Flange connections

#### Flange DIN 11864-2 Form A, female

Stainless steel: order code for "Process connection", option DQS


Suitable for pipe as per EN 10357 series A, female

DN 2 to 8 with DN 10 flanges as standard

Surface roughness:  $Ra_{max} = 0.76 \mu m$

**i** Please note the internal diameters of the measuring pipe and process connection (E) when cleaning with pigs.

DN [mm]	Pipe [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8	13 × 1.5 (DN 10)	54	37	4 × Ø9	10	10	183
15	19 × 1.5 (DN 15)	59	42	4 × Ø9	10	16	183
25	29 × 1.5 (DN 25)	70	53	4 × Ø9	10	26	183

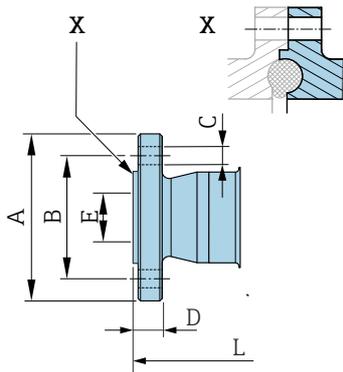

A0043232

#### Flange DIN 11864-2 Form A, flange with notch


Stainless steel: order code for "Process connection", option DRS

Suitable for pipe as per EN 10357 series A, flange with notch

Surface roughness:  $Ra_{max} = 0.76 \mu m$

**i** Please note the internal diameters of the measuring pipe and process connection (E) when cleaning with pigs.

DN [mm]	Pipe [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
40	41 × 1.5	82	65	4 × Ø9	10	38	246
50	53 × 1.5	94	77	4 × Ø9	10	50	246
65	70 × 2	113	95	8 × Ø9	10	66	246
80	85 × 2	133	112	8 × Ø11	10	81	270
100	104 × 2	159	137	8 × Ø11	10	100	278
125	129 × 2	183	161	8 × Ø11	10	125	362
150	154 × 2	213	188	8 × Ø14	10	150	362

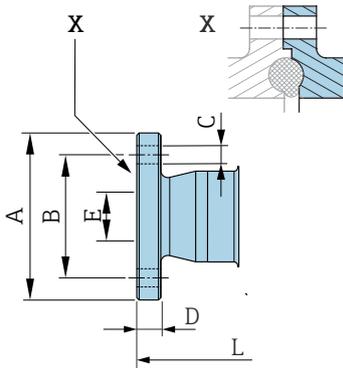


A0042819

**Flange in accordance with EN 1092-1 (DIN 2501 / DIN 2512N): PN 40**

Stainless steel: order code for "Process connection", option D5S

Surface roughness: EN 1092-1 Form B1 (DIN 2526 Form C),  $R_a \leq 1.6 \mu\text{m}$ 

DN 2 to 8 with DN 15 flanges as standard

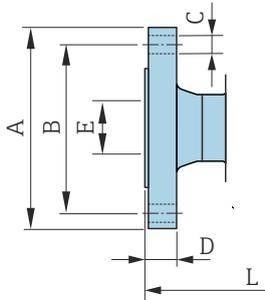

A0042813


DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8	95	65	4 × Ø14	16	17.3	198.4
15	95	65	4 × Ø14	16	17.3	198.4
25	115	85	4 × Ø14	18	28.5	198.4

**Flange according to ASME B16.5, Class 150**

Stainless steel: order code for "Process connection", option A1S

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

DN 2 to 8 with DN 15 flanges as standard



A0042813


DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8	90	60.3	4 × Ø15.7	11.2	15.7	218
15	90	60.3	4 × Ø15.7	11.2	15.7	218
25	110	79.4	4 × Ø15.7	14.2	26.7	230

**Flange according to JIS B2220, 20K**

Stainless steel: order code for "Process connection", option N4S

Surface roughness:  $Ra \leq 1.6 \mu m$

DN [mm]	A [mm]	B [mm]	C [mm]	D [mm]	E [mm]	L [mm]
2 to 8	95	70	4 × Ø15	14	15	220
15	95	70	4 × Ø15	14	15	220
25	125	90	4 × Ø19	16	25	220



A0042813

## Clamp connections


### Tri-Clamp

1.4404/316L: order code for "Process connection", option FAS

Suitable for pipe as per ASME BPE (DIN 11866 series C)

Surface roughness:  $Ra_{max} = 0.76 \mu m$

 Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.



A0043179

DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
2 to 8	12.7 × 1.65	25	9.4	143
15	19.1 × 1.65	25	15.8	143
25	25.4 × 1.65	50.4	22.1	143
40	38.1 × 1.65	50.4	34.8	220
50	50.8 × 1.65	63.9	47.5	220
65	63.5 × 1.65	77.4	60.2	220
80	76.2 × 1.65	90.9	72.9	220
100	101.6 × 2.11	118.9	97.4	220
150	152.4 × 2.77	166.9	146.9	300

### Welding socket


#### Welding socket according to EN 10357

1.4404/316L: order code for "Process connection", option DAS

Suitable for pipe EN 10357 series A

Surface roughness:  $Ra_{max} = 0.76 \mu m$

**i** Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.



DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
2 to 8	13 × 1.5	13	10	132.6
15	19 × 1.5	19	16	132.6
25	29 × 1.5	29	26	132.6
40	41 × 1.5	41	38	220
50	53 × 1.5	53	50	220
65	70 × 2	70	66	220
80	85 × 2	85	81	220
100	104 × 2	104	100	220
125	129 × 2	129	125	300
150	154 × 2	154	150	300


#### Welding socket according to ISO 2037

1.4404/316L: order code for "Process connection", option IAS

Suitable for pipe ISO 2037

Surface roughness:  $Ra_{max} = 0.76 \mu m$

**i** Please note the internal diameters of the measuring pipe and process connection (dimension B) when cleaning with pigs.



DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
2 to 8	12.7 × 1.65	12	10	118.2
15	19.05 × 1.65	18	16	118.2
25	25.4 × 1.60	25	22.6	118.2
40	38 × 1.2	38	35.6	220
50	51 × 1.2	51	48.6	220
65	63.5 × 1.6	63.5	60.3	220
80	76.1 × 1.6	76.1	72.9	220
100	101.6 × 2	101.6	97.6	220
125	139.7 × 2	139.7	135.7	380
150	168.3 × 2.6	168.3	163.1	380


**Welding socket according to ASME BPE**

1.4404/316L: order code for "Process connection", option AAS

Suitable for pipe as per ASME BPE (DIN 11866 series C)

Surface roughness:  $Ra_{max} = 0.76 \mu\text{m}$ 

 Please note the internal diameters of the measuring pipe and process connection (dimension B) when cleaning with pigs.



A0043180

DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
2 to 8	12.7 × 1.65	12.7	9	118.2
15	19.1 × 1.65	19.1	16	118.2
25	25.4 × 1.65	25.4	22.6	118.2
40	38.1 × 1.65	38.1	34.8	220
50	50.8 × 1.65	50.8	47.5	220
65	63.5 × 1.65	63.5	60.2	220
80	76.2 × 1.65	76.2	72.9	220
100	101.6 × 1.65	101.6	97.4	220
150	152.4 × 2.77	152.4	146.9	300

## Couplings

### Thread according to DIN 11851 SC


1.4404/316L: order code for "Process connection", option DCS

Suitable for pipe EN 10357 series B (DN 2 to 25)

Surface roughness:  $Ra_{max} = 0.76 \mu m$

**i** Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.

DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
2 to 8	12 × 1 (DN 10)	Rd 28 × 1/8	10	174
15	18 × 1.5 (ODT 3/4")	Rd 34 × 1/8	16	174
25	28 × 1 or 28 × 1.5	Rd 52 × 1/6	26	190



A0043253


1.4404/316L: order code for "Process connection", option DCS

Suitable for pipe EN 10357 series A (DN 40 to 150)

Surface roughness:  $Ra_{max} = 0.76 \mu m$

**i** Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.

DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
40	41 × 1.5	Rd 65 × 1/6	38	260
50	53 × 1.5	Rd 78 × 1/6	50	260
65	70 × 2	Rd 95 × 1/6	66	270
80	85 × 2	Rd 110 × 1/4	81	280
100	104 × 2	Rd 130 × 1/4	100	290
125	129 × 2	Rd 160 × 1/4	125	380
150	154 × 2	Rd 160 × 1/4	150	390



A0043253


**Thread according to DIN 11864-1, Form A**

1.4404/316L: order code for "Process connection", option DDS

Suitable for pipe EN 10357 series A

Surface roughness:  $Ra_{max} = 0.76 \mu\text{m}$ 

 Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.



DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
2 to 8	Pipe 13 × 1.5 (DN 10)	Rd 28 × 1/8	10	170
15	Pipe 19 × 1.5	Rd 34 × 1/8	16	170
25	Pipe 29 × 1.5	Rd 52 × 1/6	26	184
40	41 × 1.5	Rd 65 × 1/6	38	256
50	53 × 1.5	Rd 78 × 1/6	50	256
65	70 × 2	Rd 95 × 1/6	66	266
80	85 × 2	Rd 110 × 1/4	81	276
100	104 × 2	Rd 130 × 1/4	100	286


A0043253

**Male thread according to ISO 228/DIN 2999**

1.4404/316L: order code for "Process connection", option I2S

Suitable for female thread ISO 228/DIN 2999

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$




A0043253

DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
2 to 8	R $\frac{3}{8}$	R $10.1 \times \frac{3}{8}$	10	166
15	R $\frac{1}{2}$	R $13.2 \times \frac{1}{2}$	16	166
25	R 1	R $16.5 \times 1$	25	170

## Mounting kit

### Wall mounting kit

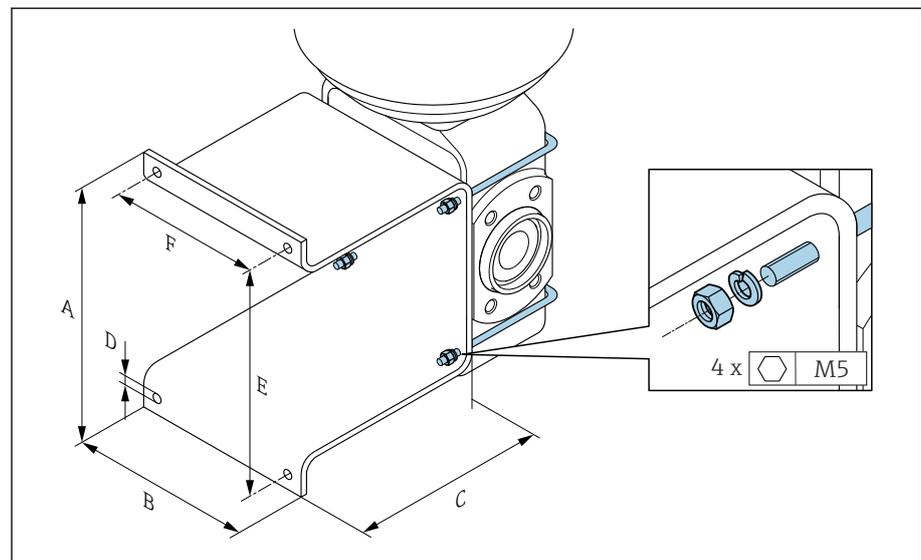

A	B	C	Ø D	E	F
[mm]	[mm]	[mm]	[mm]	[mm]	[mm]
137	110	120	7	125	88


### Accessories

#### Grounding rings

Order code: DK5HR-\*\*\*\*

1.4435 (316L), Alloy C22, tantalum

For lap joint flange made of PVDF and PVC adhesive sleeve

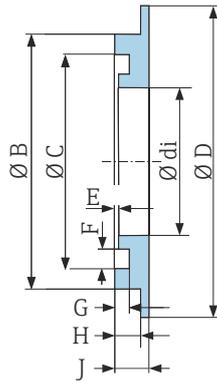


A0017673

DN [mm]	di [mm]	B [mm]	C [mm]	D [mm]	D [mm]	E [mm]	G [mm]	H [mm]	J [mm]
2 to 8	9	22	17.6	33.9	0.5	3.5	1.9	3.4	4.5
15	16	29	24.6	33.9	0.5	3.5	1.9	3.4	4.5
25	26	39	34.6	43.9	0.5	3.5	1.9	3.4	4.5

#### Spacer

Order code: DK5HB-\*\*\*\*



A0017294


DN [mm]	di [mm]	D1 [mm]	D2 [mm]	L [mm]
80	72.9	140.7	141	30
100	97.4	166.7	162	30

**Male thread with O-ring seal**

Order code: DKH\*\* -GD\*\*

1.4404/316L

Suitable for NPT female thread

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

A0043253


DN [mm]	Thread [mm]	A [mm]	B [mm]	L [mm]
2 to 8	NPT 3/8	R 15.5 × 3/8	10	186
15	NPT 1/2	R 20 × 1/2	16	186
25	NPT 1	R 25 × 1	25	196

**Female thread with O-ring seal**

Order code: DKH\*\* -GC\*\*

1.4404/316L

Suitable for NPT male thread

Surface roughness:  $R_a \leq 1.6 \mu\text{m}$ 

A0043253

DN [mm]	Thread [mm]	A [mm]	B [mm]	L [mm]
2 to 8	NPT 3/8	R 13 × 3/8	8.9	176
15	NPT 1/2	R 14 × 1/2	16	176
25	NPT 1	R 17 × 1	27.2	188

**Tri-Clamp**

Order code: DKH\*\*-HF\*\*


1.4404 (316L)

Suitable for pipe in accordance with ASME BPE (reduction)

Surface roughness: Ra<sub>max</sub> = 0.76 µm


**i** Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.

DN [mm]	Pipe [mm]	A [mm]	B [mm]	L [mm]
15	Pipe ODT 1	50.4	22.1	143



A0043179

**Protective cover**

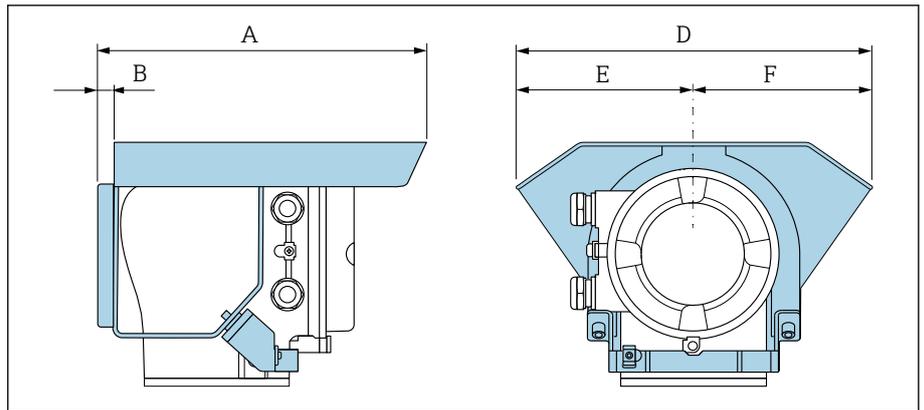

A0042332

A [mm]	B [mm]	D [mm]	E [mm]	F [mm]
257	12	280	140	140

---


## Dimensions in US units

---

<b>Compact version</b>	<b>78</b>
Order code for "Housing", option A "Aluminum, coated"	78
<b>Remote version</b>	<b>79</b>
Transmitter remote version	79
Sensor remote version	80
<b>Sensor flange connection</b>	<b>81</b>
<b>Flange connections</b>	<b>83</b>
Flange according to ASME B16.5, Class 150	83
<b>Clamp connections</b>	<b>83</b>
Tri-Clamp	83
<b>Welding socket</b>	<b>84</b>
Welding socket according to ISO 2037	84
Welding socket according to ASME BPE	84
<b>Mounting kits</b>	<b>85</b>
Wall mounting kit	85
<b>Accessories</b>	<b>86</b>
Spacer	86
Clamp connections with aseptic gasket seal available for order	86
Threaded glands with O-ring seal available for order	87
Grounding rings	88
Protective cover	88

## Compact version

Order code for "Housing", option A "Aluminum, coated"

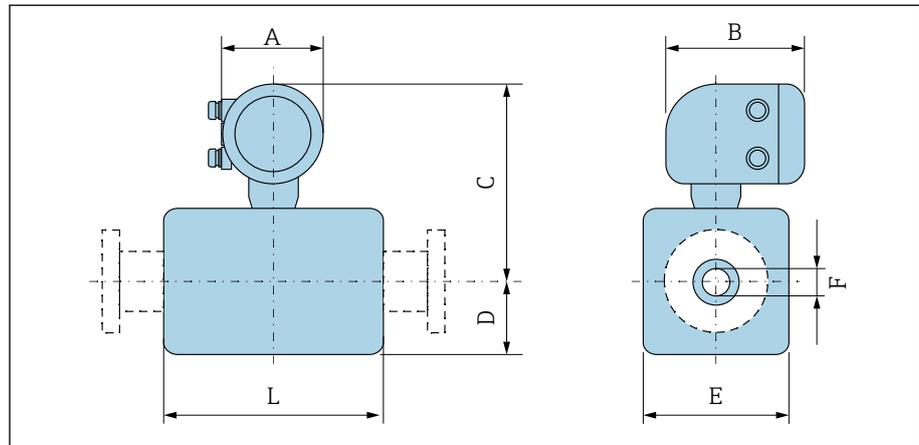

A0043172


DN		A <sup>1)</sup>	B	C	D	E	F	L <sup>2)</sup>
[mm]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]
2	1/12	5.47	7.01	9.25	1.89	1.69	0.089	3.39
4	1/32	5.47	7.01	9.25	1.89	1.69	0.18	3.39
8	5/16	5.47	7.01	9.25	1.89	1.69	0.35	3.39
15	1/2	5.47	7.01	9.25	1.89	1.69	0.63	3.39
-	1	5.47	7.01	9.41	2.05	2.2	0.89	3.39
25	-	5.47	7.01	9.41	2.05	2.2	1.02	3.39
40	1 1/2	5.47	7.01	9.53	2.13	4.21	1.37	5.51
50	2	5.47	7.01	9.8	2.36	4.72	1.87	5.51
65	-	5.47	7.01	10.08	2.68	5.31	2.37	5.51
80	3	5.47	7.01	10.35	2.91	5.83	2.87	5.51
100	4	5.47	7.01	10.87	3.43	6.85	3.83	5.51
125	-	5.47	7.01	11.5	4.06	8.11	4.72	7.87
150	6	5.47	7.01	12.05	4.61	9.21	5.78	7.87

1) Depending on the cable gland used: values up to +1.18 in

2) Total length depends on the process connections.

### Remote version

#### Transmitter remote version

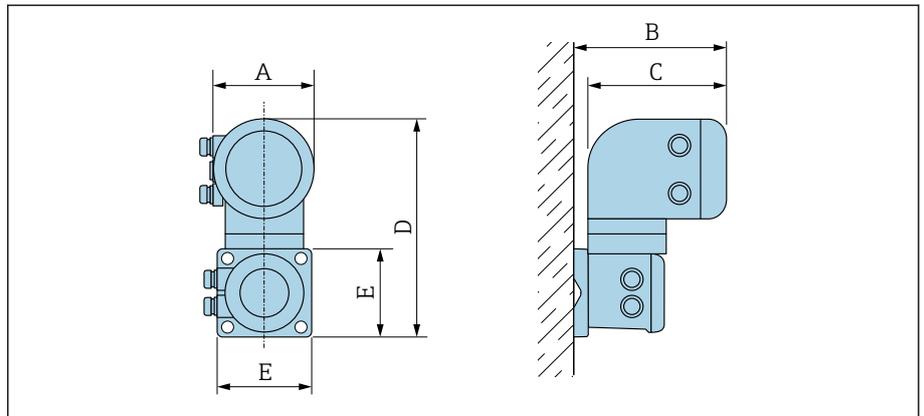


A0042715

Order code for "Housing"	A <sup>1)</sup> [in]	B [in]	C [in]	D [in]	E [in]
Option P "Remote, aluminum, coated"	5.47	7.28	7.01	12.17	5.12

1) Depending on the cable entry used: values up to +1.18 in

## Sensor remote version

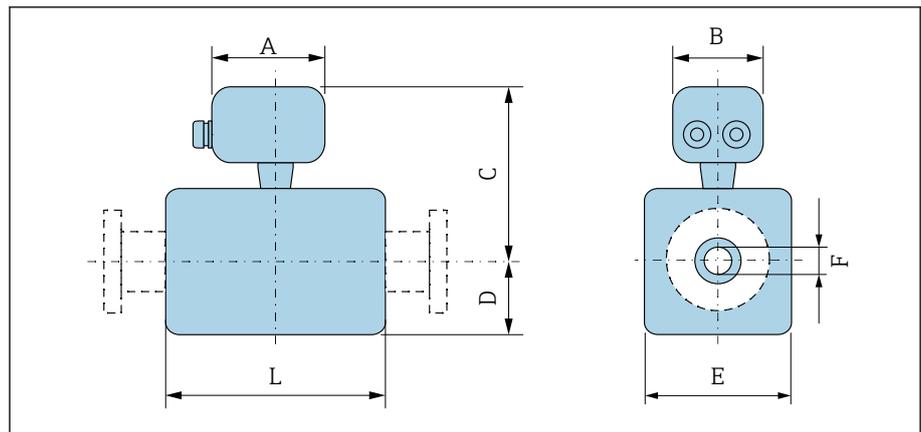


A0043178

[mm]	DN		A <sup>1)</sup>	B	C	D	E	F	L <sup>2)</sup>
	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]	[in]
2		1/12	7.2	8.15	5.08	2.17	1.69	0.089	3.39
4		1/32	7.2	8.15	5.08	2.17	1.69	0.18	3.39
8		5/16	7.2	8.15	5.08	2.17	1.69	0.35	3.39
15		1/2	7.2	8.15	5.08	2.17	1.69	0.63	3.39
-		1	7.2	8.15	5.24	2.17	2.2	0.89	3.39
25		-	7.2	8.15	5.24	2.17	2.2	1.02	3.39
40		1 1/2	7.2	8.15	5.35	2.13	4.21	1.37	5.51
50		2	7.2	8.15	5.63	2.36	4.72	1.87	5.51
65		-	7.2	8.15	5.91	2.64	5.31	2.37	5.51
80		3	7.2	8.15	6.18	2.91	5.83	2.87	5.51
100		4	7.2	8.15	6.69	3.43	6.85	3.83	5.51
125		-	7.2	8.15	7.32	4.06	8.11	4.72	7.87
150		6	7.2	8.15	7.87	4.61	9.21	5.78	7.87

1) Depending on the cable gland used: values up to +1.18 in

2) Total length depends on the process connections.


Sensor flange connection

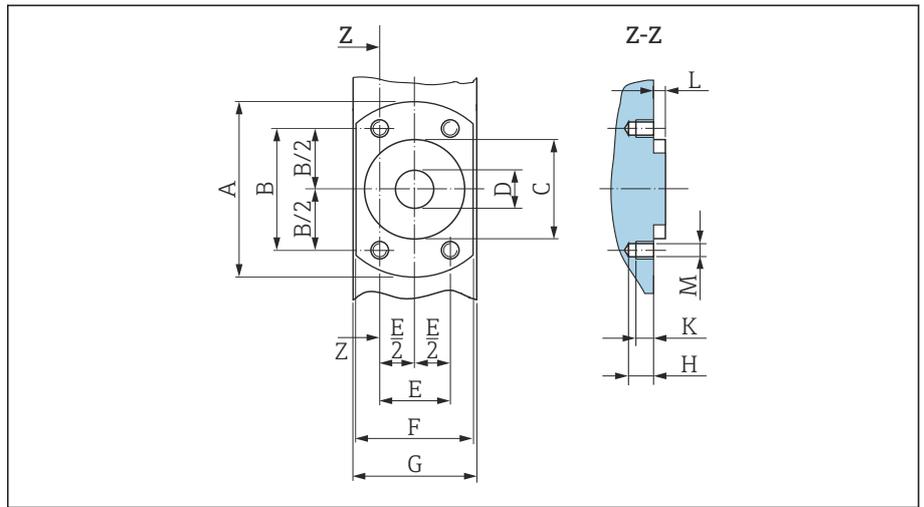

A0017657

7 Front view without process connections

DN		A	B	C	D	E	F	G	H	K	L	M
[mm]	[in]	[mm]										
2	1/12	2.44	1.64	1.34	0.35	0.94	1.65	1.69	0.33	0.24	0.16	M6
4	1/32	2.44	1.64	1.34	0.35	0.94	1.65	1.69	0.33	0.24	0.16	M6
8	5/16	2.44	1.64	1.34	0.35	0.94	1.65	1.69	0.33	0.24	0.16	M6
15	1/2	2.44	1.64	1.34	0.63	0.94	1.65	1.69	0.33	0.24	0.16	M6
25	-	2.83	1.98	1.73	1.02	1.14	2.17	2.2	0.33	0.24	0.16	M6

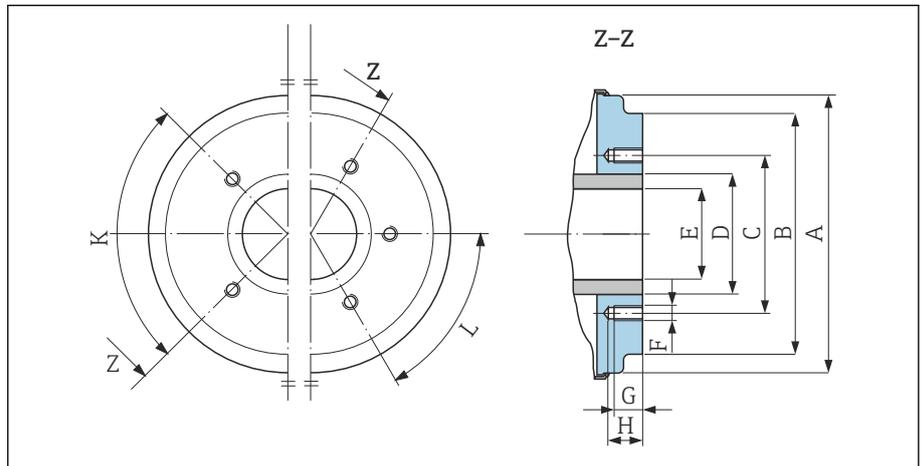

A0005528

8 Front view without process connections

DN		A	B	C	D	E	F	G	H	K	L
[mm]	[in]	[in]	[in]	[in]	[in]	[in]	[mm]	[in]	[in]	90° ±0.5°	60° ±0.5°
											Tapped holes
40	1 1/2	3.93	3.38	2.8	1.9	1.37	M8	0.47	0.67	4	-
50	2	4.44	3.89	3.29	2.37	1.87	M8	0.47	0.67	4	-
65	-	5.03	4.52	3.94	3	2.37	M8	0.47	0.67	-	6
80	3	5.54	5.26	4.49	3.5	2.87	M8	0.47	0.67	-	6

DN		A	B	C	D	E	F	G	H	K	L
[mm]	[in]	[in]	[in]	[in]	[in]	[in]	[mm]	[in]	[in]	90° ±0.5°	60° ±0.5°
		Tapped holes									
100	4	6.56	6.28	5.55	4.5	3.83	M8	0.47	0.67	-	6
125	-	7.82	7.54	6.73	5.5	4.72	M10	0.59	0.79	-	6
150	6	8.93	8.64	7.87	6.63	5.78	M10	0.59	0.79	-	6


## Flange connections

### Flange according to ASME B16.5, Class 150

Stainless steel: order code for "Process connection", option A1S

Surface roughness:  $R_a \leq 63 \mu\text{m}$

DN  $\frac{1}{12}$ " to  $\frac{5}{16}$ " with DN  $\frac{1}{2}$ " flanges as standard



DN [in]	A [in]	B [in]	C [in]	D [in]	E [in]	L [in]
$\frac{1}{12}$ to $\frac{5}{16}$	3.54	2.37	4 × Ø0.62	0.44	0.62	8.58
$\frac{1}{2}$	3.54	2.37	4 × Ø0.62	0.44	0.62	8.58
1	4.33	3.13	4 × Ø0.62	0.56	1.05	9.06

A0042813

## Clamp connections


### Tri-Clamp

1.4404/316L: order code for "Process connection", option FAS

Suitable for pipe as per ASME BPE (DIN 11866 series C)

Surface roughness:  $R_{a_{\text{max}}} = 30 \mu\text{m}$

**i** Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.



DN [in]	Pipe [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{5}{16}$	0.5 × 0.065	0.98	0.37	5.63
$\frac{1}{2}$	0.75 × 0.065	0.98	0.62	5.63
1	1 × 0.065	1.98	0.87	5.63
1 ½	1.5 × 0.065	1.98	1.37	8.66
2	2 × 0.065	2.52	1.87	8.66
3	3 × 0.065	3.58	2.87	8.66
4	4 × 0.083	4.68	3.83	8.66
6	6 × 0.109	6.57	5.78	11.81

A0043179

## Welding socket


### Welding socket according to ISO 2037

1.4404/316L: order code for "Process connection", option IAS

Suitable for pipe ISO 2037

Surface roughness:  $Ra_{max} = 30 \mu\text{in}$

 Please note the internal diameters of the measuring pipe and process connection (dimension B) when cleaning with pigs.



A0043180

DN [in]	Pipe [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{5}{16}$	$0.5 \times 0.065$	0.47	0.39	4.65
$\frac{1}{2}$	$0.75 \times 0.065$	0.71	0.63	4.65
1	$1 \times 0.06$	0.98	0.89	4.65
1 $\frac{1}{2}$	$38 \times 0.05$	1.5	1.4	8.66
2	$51 \times 0.05$	2.01	1.91	8.66
3	$3 \times 0.06$	3	2.87	8.66
4	$4 \times 0.08$	4	3.84	8.66
5	$5.5 \times 0.08$	5.5	5.34	14.96
6	$6.63 \times 0.1$	6.63	6.42	14.96


### Welding socket according to ASME BPE

1.4404/316L: order code for "Process connection", option AAS

Suitable for pipe as per ASME BPE (DIN 11866 series C)

Surface roughness:  $Ra_{max} = 30 \mu\text{in}$

 Please note the internal diameters of the measuring pipe and process connection (dimension B) when cleaning with pigs.




A0043180

DN [in]	Pipe [in]	A [in]	B [in]	L [in]
$\frac{1}{12}$ to $\frac{5}{16}$	$0.5 \times 0.065$	0.5	0.35	4.65
$\frac{1}{2}$	$0.75 \times 0.065$	0.75	0.63	4.65
1	$1 \times 0.065$	1	0.89	4.65
1 $\frac{1}{2}$	$1.5 \times 0.065$	1.5	1.37	8.66
2	$2 \times 0.065$	2	1.87	8.66
3	$3 \times 0.065$	3	2.87	8.66
4	$4 \times 0.065$	4	3.83	8.66
6	$6 \times 0.109$	6	5.78	11.81

## Mounting kits

### Wall mounting kit

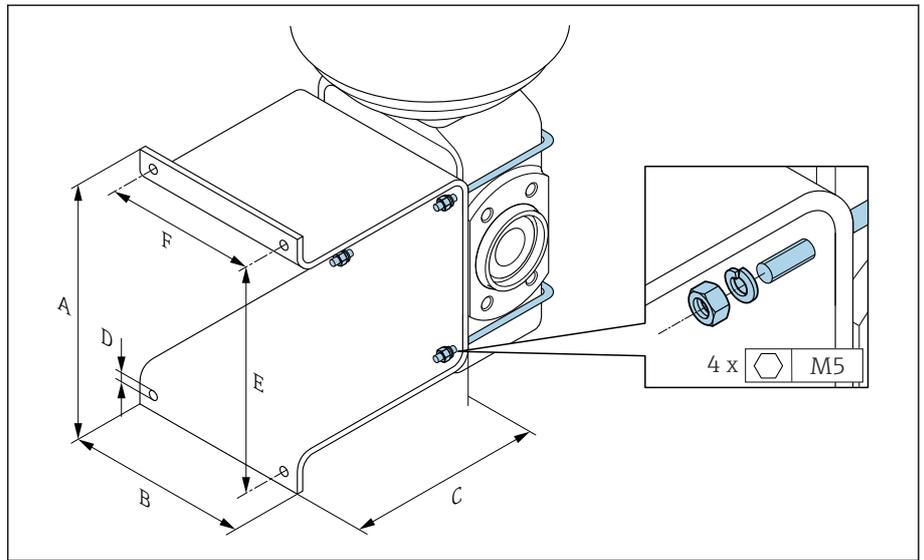


A000537

A	B	C	Ø D	E	F
[in]	[in]	[in]	[in]	[in]	[in]
5.39	4.33	4.72	0.28	4.92	3.46

## Accessories

### Spacer

Order code: DK5HB-\*\*\*\*



A0017294

DN [in]	di [in]	D1 [in]	D2 [in]	L [in]
3	2.87	5.54	5.55	1.30
4	3.83	6.56	6.38	1.30

### Clamp connections with aseptic gasket seal available for order


Order code: DKH\*\*-HF\*\*

1.4404 (316L)

Suitable for pipe in accordance with ASME BPE (reduction)

Surface roughness:  $Ra_{max} = 30 \mu\text{in}$


 Please note the internal diameters of the measuring pipe and process connection (B) when cleaning with pigs.



A0043179

DN [in]	Pipe [in]	A [in]	B [in]	L [in]
½	Pipe ODT 1	1.98	0.87	5.63

Threaded glands with O-ring seal available for order

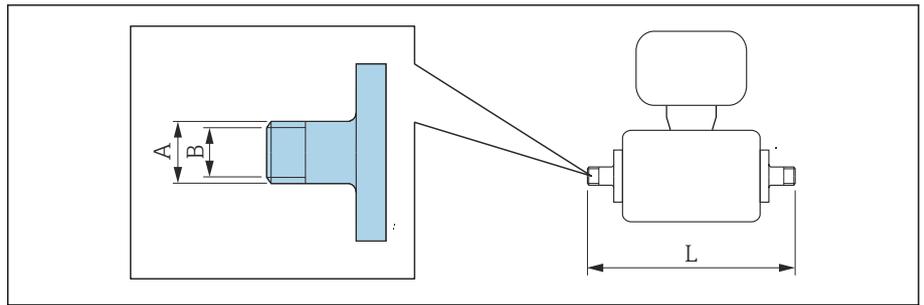

A0027509

**Male thread**  
**1.4404 (316L)**  
**Order code: DKH\*\*GD\*\***

DN [in]	Suitable for NPT female thread [in]	A [in]	B [in]	L [in]
1/12 to 3/8	NPT 3/8	R 0.61 × 3/8	0.39	7.39
1/2	NPT 1/2	R 0.79 × 1/2	0.63	7.39
1	NPT 1	R 1 × 1	1.00	7.73

Surface roughness: Ra ≤ 63 µin

**Female thread**  
**1.4404 (316L)**  
**Order code: DKH\*\*GC\*\***

DN [in]	Suitable for NPT male thread [in]	A [in]	B [in]	L [in]
1/12 to 3/8	NPT 3/8	R 0.51 × 3/8	0.35	6.93
1/2	NPT 1/2	R 0.55 × 1/2	0.63	6.93
1	NPT 1	R 0.67 × 1	1.07	7.41


Surface roughness: Ra ≤ 63 µin

**Grounding rings**

Order code: DK5HR-\*\*\*\*

1.4435 (316L), Alloy C22, tantalum


For lap joint flange made of PVDF and PVC adhesive sleeve

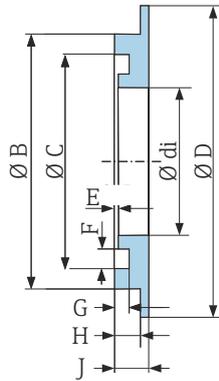

A0017673

DN [in]	di [in]	B [in]	C [in]	D [in]	D [in]	E [in]	G [in]	H [in]	J [in]
1/12 to 3/8	0.35	0.87	0.69	1.33	0.02	0.14	0.07	0.13	0.18
1/2	0.63	1.14	0.97	1.33	0.02	0.14	0.07	0.13	0.18
1	0.89	1.44	1.23	1.73	0.02	0.14	0.07	0.13	0.18

**Protective cover**

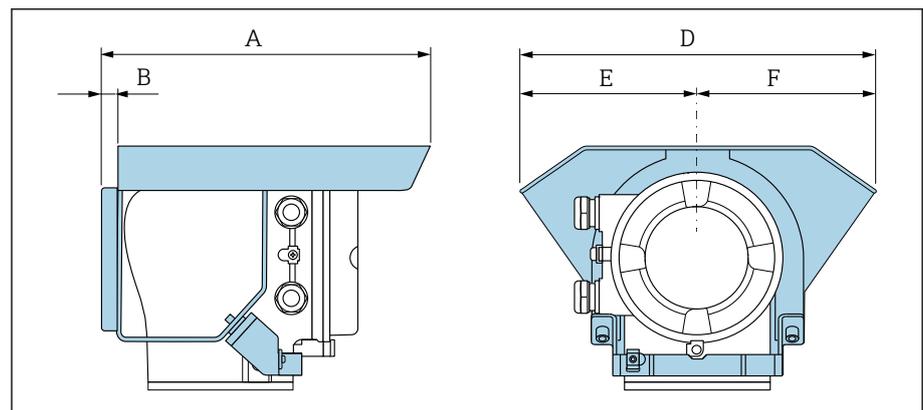

A0042332

A [in]	B [in]	D [in]	E [in]	F [in]
10.12	0.47	11.02	5.51	5.51

## Local display

---

Operating concept	90
Operating options	90
Operating tools	91

## Operating concept

Operation method	<ul style="list-style-type: none"> <li>Operation via local display with touch screen.</li> <li>Operation via SmartBlue App.</li> </ul>
Menu structure	<p>Operator-oriented menu structure for user-specific tasks:</p> <ul style="list-style-type: none"> <li>Diagnostics</li> <li>Application</li> <li>System</li> <li>Guidance</li> <li>Language</li> </ul>
Commissioning	<ul style="list-style-type: none"> <li>Commissioning via a guided menu (<b>Commissioning</b> wizard).</li> <li>Menu guidance with interactive help function for individual parameters.</li> </ul>
Reliable operation	<ul style="list-style-type: none"> <li>Operation in local language.</li> <li>Uniform operating philosophy in device and in the SmartBlue App.</li> <li>Write protection</li> <li>When electronics modules are replaced: configurations are transferred using the T-DAT Backup device memory. The device memory contains process data, device data and the event logbook. No reconfiguration is necessary.</li> </ul>
Diagnostic behavior	<p>Efficient diagnostic behavior increases measurement availability:</p> <ul style="list-style-type: none"> <li>Open troubleshooting measures via local display and SmartBlue App.</li> <li>Diverse simulation options.</li> <li>Logbook of events that have occurred.</li> </ul>

## Operating options

Local display	 <p>Display elements:</p> <ul style="list-style-type: none"> <li>LCD touch screen</li> <li>Depends on the orientation, automatic alignment of local display.</li> <li>Configuration of display format for measured variables and status variables.</li> </ul> <p>Operating elements:</p> <ul style="list-style-type: none"> <li>Touch screen</li> <li>Local display can also be accessed in the hazardous area.</li> </ul>
SmartBlue App	<ul style="list-style-type: none"> <li>The SmartBlue App allows the user to put devices into operation and operate them.</li> <li>Based on Bluetooth.</li> <li>No separate driver required.</li> <li>Available for mobile handheld terminals, tablets and smartphones.</li> <li>Suitable for convenient and secure access to devices in hard-to-reach locations or in hazardous areas.</li> <li>Can be used within a 20 m (65.6 ft) radius of the device.</li> <li>Encrypted and secure data transmission.</li> <li>No data loss during commissioning and maintenance.</li> <li>Diagnostic information and process information in real time.</li> </ul>

## Operating tools

Operating tools	Operating unit	Interface	Additional information
DeviceCare SFE100	<ul style="list-style-type: none"> <li>▪ Notebook</li> <li>▪ PC</li> <li>▪ Tablet with Microsoft Windows system</li> </ul>	<ul style="list-style-type: none"> <li>▪ CDI service interface</li> <li>▪ Fieldbus protocol</li> </ul>	Innovation brochure IN01047S
FieldCare SFE500	<ul style="list-style-type: none"> <li>▪ Notebook</li> <li>▪ PC</li> <li>▪ Tablet with Microsoft Windows system</li> </ul>	<ul style="list-style-type: none"> <li>▪ CDI service interface</li> <li>▪ Fieldbus protocol</li> </ul>	Operating Instructions BA00027S and BA00059S
SmartBlue App	<ul style="list-style-type: none"> <li>▪ Devices with iOS: iOS9.0 or higher</li> <li>▪ Devices with Android: Android 4.4 KitKat or higher</li> </ul>	Bluetooth	Endress+HauserSmartBlue App: <ul style="list-style-type: none"> <li>▪ Google Playstore (Android)</li> <li>▪ iTunes Apple Shop (iOS devices)</li> </ul>
Device Xpert	Field Xpert SFX 100/350/370	HART fieldbus protocol	Operating Instructions BA01202S

---

## Certificates and approvals

---

Non-Ex approval	94
Pressure Equipment Directive	94
Pharmaceutical compatibility	94
HART certification	94
Radio approval	94
Other standards and guidelines	94

### Non-Ex approval

- cSAus
- EAC

### Pressure Equipment Directive

- CRN
- PED Cat. II/III

### Pharmaceutical compatibility

- FDA
- USP Class VI
- TSE/BSE Certificate of Suitability
- cGMP

### HART certification

The device is certified and registered by the FieldComm Group. The measuring system meets all the requirements of the following specifications:

- Certified according to HART 7
- The device can also be operated with certified devices of other manufacturers (interoperability).

### Radio approval

The device has radio approvals.

### Other standards and guidelines

- IEC/EN 60529  
Degrees of protection provided by enclosures (IP code)
- IEC/EN 60068-2-6  
Environmental influences: Test procedure - Test Fc: vibrate (sinusoidal)
- IEC/EN 60068-2-31  
Environmental influences: Test procedure - Test Ec: shocks due to rough handling, primarily for devices.
- IEC/EN 61010-1  
Safety requirements for electrical equipment for measurement, control and laboratory use - general requirements.
- CAN/CSA-C22.2 No. 61010-1-12  
Safety Requirements for Electrical Equipment for Measurement, Control and Laboratory Use - Part 1 General Requirements.
- IEC/EN 61326  
Emission in accordance with Class A requirements. Electromagnetic compatibility (EMC requirements)
- ANSI/ISA-61010-1 (82.02.01)  
Safety Requirements for Electrical Equipment for Measurement, Control and Laboratory Use - Part 1 General Requirements.
- NAMUR NE 21  
Electromagnetic compatibility (EMC) of industrial process and laboratory control equipment.
- NAMUR NE 32  
Data retention in the event of a power failure in field and control instruments with microprocessors.
- NAMUR NE 43  
Standardization of the signal level for the breakdown information of digital transmitters with analog output signal.
- NAMUR NE 53  
Software of field devices and signal-processing devices with digital electronics.
- NAMUR NE 105  
Specifications for integrating fieldbus devices in engineering tools for field devices.
- NAMUR NE 107  
Self-monitoring and diagnosis of field devices.

- NAMUR NE 131  
Requirements for field devices for standard applications.
- ETSI EN 300 328  
Guidelines for 2.4 GHz radio components
- EN 301489  
Electromagnetic compatibility and radio spectrum matters (ERM).

---

## Application packages

---

Use	98
Heartbeat Verification + Monitoring	98

## Use

Many different application packages are available to enhance the functionality of the device. Such packages might be needed to address safety aspects or specific application requirements.

The application packages can be ordered with the device or subsequently from Endress+Hauser. Detailed information on the relevant order code is available from your local Endress+Hauser sales organization or on the product page of the Endress+Hauser website: [www.endress.com](http://www.endress.com).

## Heartbeat Verification + Monitoring

### Heartbeat Verification

Availability depends on the product structure.

Meets the requirement for traceable verification to DIN ISO 9001:2008 Chapter 7.6 a) "Control of monitoring and measuring equipment":

- Functional testing in the installed state without interrupting the process.
- Traceable verification results on request, including a report.
- Simple testing process with local operation or other operating interfaces.
- Clear measuring point assessment (pass/fail) with high test coverage within the framework of manufacturer specifications.
- Extension of calibration intervals according to operator's risk assessment.

### Heartbeat Monitoring

Availability depends on the product structure.

Heartbeat Monitoring continuously supplies data, which are characteristic of the measuring principle, to an external condition monitoring system for the purpose of preventive maintenance or process analysis. These data enable the operator to:

- Draw conclusions - using these data and other information - about the impact the process influences, e.g. corrosion, abrasion, formation of buildup, have on the measuring performance over time.
- Schedule servicing in time.
- Monitor the process quality or product quality, e.g. gas pockets.

## Accessories

---

Device-specific accessories	100
Communication-specific accessories	101
Service-specific accessory	101
System components	102

## Device-specific accessories

### Transmitter

Accessories	Description	Order number
Proline 10 transmitter	 Installation Instructions EA01350D	5XBBXX-*...*
Protective cover	Protects the device from weather exposure:  Installation Instructions EA01351D	71502730
Connecting cable	Can be ordered with the device. The following cable lengths are available: order code for "Cable, sensor connection" <ul style="list-style-type: none"> <li>▪ 5 m (16 ft)</li> <li>▪ 10 m (32 ft)</li> <li>▪ 20 m (65 ft)</li> <li>▪ User-configurable cable length (m or ft)</li> </ul>  Max. cable length: 200 m (660 ft)	DK5013-*...*

### Sensor

Accessories	Description
Adapter set	Adapter connections for installing a Promag H instead of a Promag 30/33 A or Promag 30/33 H (DN 25). Consists of: <ul style="list-style-type: none"> <li>▪ 2 process connections</li> <li>▪ Screws</li> <li>▪ Seals</li> </ul>
Seal set	Replacement of seals
Spacer	A spacer is needed if an installed device with DN 80 or DN 100 must be replaced and the new sensor is shorter.
Welding jig	Welding socket as process connection: welding jig for installation in pipe.
Grounding rings	Ground medium in lined measuring pipes.  Installation Instructions EA00070D
Grounding rings	Ground medium in lined measuring pipes.  Installation Instructions EA00070D
Wall mounting kit	Wall mounting kit (only DN 2 to 25 (1/12 to 1"))
Mounting kit	Consists of: <ul style="list-style-type: none"> <li>▪ 2 process connections</li> <li>▪ Screws</li> <li>▪ Seals</li> </ul>

## Communication-specific accessories

Accessories	Description
Commubox FXA195 USB/HART modem	Intrinsically safe HART communication with FieldCare and FieldXpert  Technical Information TI00404F
Commubox FXA291	Connects the Endress+Hauser devices with the CDI interface (= Endress+Hauser Common Data Interface) to the USB interface of a personal computer or laptop.  Technical Information TI405C/07
HART Loop Converter HMX50	Is used to evaluate and convert dynamic HART process variables to analog current signals or limit values.  <ul style="list-style-type: none"> <li>▪ Technical Information TI00429F</li> <li>▪ Operating Instructions BA00371F</li> </ul>
Fieldgate FXA42	Transmission of measured values from connected 4 to 20 mA analog and digital devices.  <ul style="list-style-type: none"> <li>▪ Technical Information TI01297S</li> <li>▪ Operating Instructions BA01778S</li> <li>▪ Product page: <a href="http://www.endress.com/fxa42">www.endress.com/fxa42</a></li> </ul>
Field Xpert SMT70	Tablet PC for the configuration of the device. Enables mobile Plant Asset Management to manage the devices with a digital communication interface. Suitable for Zone 2.  <ul style="list-style-type: none"> <li>▪ Technical Information TI01342S</li> <li>▪ Operating Instructions BA01709S</li> <li>▪ Product page: <a href="http://www.endress.com/smt70">www.endress.com/smt70</a></li> </ul>
Field Xpert SMT77	Tablet PC for the configuration of the device. Enables mobile Plant Asset Management to manage the devices with a digital communication interface. Suitable for Zone 1.  <ul style="list-style-type: none"> <li>▪ Technical Information TI01418S</li> <li>▪ Operating Instructions BA01923S</li> <li>▪ Product page: <a href="http://www.endress.com/smt77">www.endress.com/smt77</a></li> </ul>

## Service-specific accessory

Accessories	Description	Order number
Applicator	Software for selecting and sizing Endress+Hauser devices.	<a href="https://portal.endress.com/webapp/applicator">https://portal.endress.com/webapp/applicator</a>
W@M Life Cycle Management	<ul style="list-style-type: none"> <li>▪ Information platform with software applications and services</li> <li>▪ Supports the entire life cycle of the facility.</li> </ul>	<a href="http://www.endress.com/lifecyclemanagement">www.endress.com/lifecyclemanagement</a>
FieldCare	FDT-based plant asset management software from Endress+Hauser. Management and configuration of Endress+Hauser devices.  Operating Instructions BA00027S and BA00059S	<ul style="list-style-type: none"> <li>▪ Device driver: <a href="http://www.endress.com">www.endress.com</a> → Download Area</li> <li>▪ CD-ROM (contact Endress+Hauser)</li> <li>▪ DVD (contact Endress+Hauser)</li> </ul>
DeviceCare	Software for connecting and configuring Endress+Hauser devices.  Innovation brochure IN01047S	<ul style="list-style-type: none"> <li>▪ Device driver: <a href="http://www.endress.com">www.endress.com</a> → Download Area</li> <li>▪ CD-ROM (contact Endress+Hauser)</li> <li>▪ DVD (contact Endress+Hauser)</li> </ul>

## System components

Accessories	Description
Memograph M	Graphic data manager: <ul style="list-style-type: none"><li>▪ Record measured values</li><li>▪ Monitor limit values</li><li>▪ Analyze measuring points</li></ul>  <ul style="list-style-type: none"><li>▪ Technical Information TI00133R</li><li>▪ Operating Instructions BA00247R</li></ul>
iTEMP	Temperature transmitter: <ul style="list-style-type: none"><li>▪ Measure the absolute pressure and gauge pressure of gases, vapors and liquids</li><li>▪ Read the medium temperature</li></ul>  "Fields of Activity" document FA00006T

---



[www.addresses.endress.com](http://www.addresses.endress.com)

---